

State of North Dakota     )  
  )ss  
County of Burleigh        )

I, Charles E. Eder, do hereby certify that I am the duly-appointed State Toxicologist for the State of North Dakota and an official custodian of the records and files of the office thereof, that I have carefully compared the

**Ethanol Breath Standard Analytical Report, Lot No. 09313080A1, Expiration 06/01/2015**  
**(06/03/13)**

hereto attached with the respective original as the same appears of record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, and find the same to be a true and correct copy thereof and of the whole thereof. In witness whereof I have set my hand at the city of Bismarck, in said county this:

3<sup>rd</sup> day of JUNE, 2013


  
\_\_\_\_\_  
Charles E. Eder, State Toxicologist


State of North Dakota     )  
  )ss  
County of Burleigh        )

On this 3<sup>rd</sup> day of June, 2013, before me personally appeared Charles E. Eder, known to me to be the State Toxicologist for the State of North Dakota, and acknowledged to me that he/she has executed the same.

Subscribed to and sworn before me this:

3<sup>rd</sup> day of June, 2013

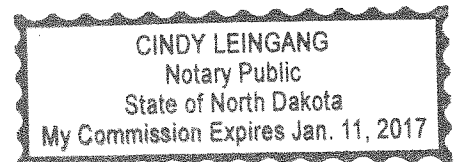

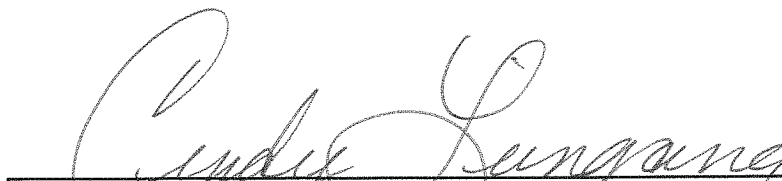  
\_\_\_\_\_  
Cindy Leingang, Notary Public, State of North Dakota  
My Commission Expires January 11, 2017

(SEAL)

## ETHANOL BREATH STANDARD ANALYTICAL REPORT

Ethanol Breath Standard Lot Number **09313080A1** Expiration Date **06-01-15**

This standard was analyzed by ILMO Specialty Gases with a reported result of 208.4 ppm which is the equivalent of 0.080 AC of Ethanol in Nitrogen. ILMO Specialty Gases has provided a Certificate of Analysis traceable to N.I.S.T. SRM Ethanol Standards.


A proper result for the standard test using a cylinder of this lot number would be the range of 0.075 to 0.085 g ethanol/210 L of vapor (g/100 ml of blood or g/210 L of end expiratory breath).

The Intoxilyzer® will print out the value of the standard test in 3 digits on Intoxilyzer® Test Record (Form 106-I8000).

The number of cylinders sent to each location will be based on need. The standard may be used until the date of expiration as indicated by the manufacturer's Certificate of Analysis.

  
\_\_\_\_\_  
Charles E. Eder, State Toxicologist

03 JUN 13  
\_\_\_\_\_  
Date Approved

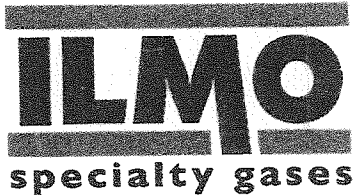

7 Eastgate Dr. • P.O. Box 790 • Jacksonville, IL 62651-0790  
217-245-2183 • Fax: 217-243-7634 • www.ilmoproducts.com

## Certificate of Analysis

Certificate ID: 4789  
Part #: BAC105L080T  
Cylinder Size: 105L  
Lot Number: 09313080A1  
Expiration: 6/1/2015

### 0.080 BAC (For use with breath alcohol testing instruments)

Contents: 105 Liters @ 1000 psig 70°F (21°C)

Component:	Concentration:	Accuracy:	Method:
Ethanol	208.4 ppm	+/- 0.002 or 2%	NDIR
Nitrogen	Balance	BAC whichever is greater	

\*NIST Standard Reference Material  
Cylinder No. CCI57791 / Job No. 13029  
Certified 184.3  $\mu\text{mol/mol}$  Ethanol in Nitrogen  
for ILMO Products Co., Jacksonville, IL

*Jacob Matthes*  
Specialty Gas Lab Tech

*05/01/13*  
Date

Distributed by: CMI Inc.  
316 East Ninth Street  
Owensboro, KY 42303  
Phone 866-835-0690  
[www.alcoholtest.com](http://www.alcoholtest.com)

