

INTOXILYZER 8000 INSPECTION

Serial No.: 80-004188

Location: Cavalier Co

- | | Check When Done |
|---|-----------------|
| A. Is the warm-up time less than 20 minutes? | <u>✓</u> |
| B. Is a three-pronged grounded outlet used? | <u>✓</u> |
| C. Is the breath tube heated? | <u>✓</u> |
| D. Is the diagnostic check complete? | <u>✓</u> |
| E. Is the time, date, and year correct (re-set if necessary)? | <u>✓</u> |
| F. Print test. (Attach test record.) | <u>✓</u> |
| G. Low AC. Use <0.03 AC in ACA mode. (Attach test record.)
Sim SN <u>DR5135</u> Lot No. <u>—</u> Rep AC <u>0.021 AC</u> | <u>✓</u> |
| H. Linearity Test. Use ≥ 0.25 AC in ACA mode. (Attach test record.)
Sim SN <u>DR3375</u> Lot No. <u>—</u> Rep AC <u>0.292 AC</u> | <u>✓</u> |
| I. Interferent check. Use 0.05% acetone plus 0.10 AC ethanol in ABA mode.
(Attach test record.)
Sim SN <u>DR5186</u> Lot No. <u>—</u> Rep AC <u>0.10 AC + Acetone (0.05%)</u> | <u>✓</u> |
| J. RFI check. Run CMS mode. Key radio on first room air.
(Attach test record.) | <u>✓</u> |
| K. Calibration Check. Use Ethanol Breath Standard cylinder. Do three sets in ACA mode.
(Attach test record.) | |

Lot No. <u>659358</u>	Cyl No. <u>53</u>	Exp. Date <u>09/03/2011</u>
Test 1 <u>0.077</u>	Test 4 <u>0.077</u>	Test 7 <u>0.077</u>
Test 2 <u>0.077</u>	Test 5 <u>0.077</u>	Test 8 <u>0.076</u>
Test 3 <u>0.077</u>	Test 6 <u>0.077</u>	Test 9 <u>0.077</u>
Average <u>0.077 AC</u>		

L. Tank pressure, Level 3 Func D Sub G P: 1015 psi Reg 625 psi

M. Remarks/Maintenance record: Annual Inspection

<u>11 May 2010</u> Date	<u>Mary Pearson</u> Field Inspector's Signature
<u>15 May 2010</u> Date	<u>Deb Kashner</u> Reviewed by

80-004188
P. 80/88 PM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004188
Location = LANG 8164.13.00 06/09
05/11/2010 14:08

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 659358
Standard Cyl #? 53
Standard Expiration? 09/03/2011
Oper No? 107501

Flow Cal. Date: 06/04/2009
Slope 689
Intercept -630047

IR Calibration Date: 12/11/2009
 3um 9um

0th Coef(*100): -36132 -37983
1st Coef(*100): 283422 138305
2nd Coef(*100): -135 610
H2O adj(mg/l*10k): 688 672

***** Printer Test End *****



Operator Signature
MARGY PEARSON

Remarks:

Print

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004188
Location = LANG 8164.13.00 06/09
05/11/2010 14:19

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:20
02 Std. Sol.	0.016	14:21
03 Room Air	0.000	14:22
04 Std. Sol.	0.016	14:22
05 Room Air	0.000	14:23
06 Std. Sol.	0.016	14:24
07 Room Air	0.000	14:24


08 Sim Temp = 34.0°C

Simul Ser No = 0000000

Std Sol No = 000000

County = 10

Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

Low AC 0.021 AC

Form 106-I8000

80-004188
P. 82/88 FA

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004188
Location = LANG 8164.13.00 06/09
05/11/2010 14:36

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:36
02 Std. Sol.	0.282	14:38
03 Room Air	0.000	14:38
04 Std. Sol.	0.282	14:39
05 Room Air	0.000	14:39
06 Std. Sol.	0.283	14:40
07 Room Air	0.000	14:41

08 Sim Temp = 34.0°C

Simul Ser No = 0000000
Std Sol No = 000000
County = 10 Oper No. = 107501

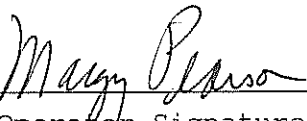

Operator Signature
MARGY PEARSON

Remarks:

Linearity 0.292 AC

Form 106-I8000

80-004188
P. 8/3/88 PM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004188
Location = LANG 8164.13.00 06/09
05/11/2010 14:11

Test	AC	Time
01 Room Air	0.000	14:12
02 *Subject Test	INT*	14:13
03 Room Air	0.000	14:13

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Simul Ser No = 0000000
Std Sol No = 000000
County = 10 Oper No. = 107501

Margy Pearson

Operator Signature
MARGY PEARSON

Remarks:

Interferent - AC + Acetone

Form 106-I8000

80-004188
P. 84/88 FM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004188
Location = LANG 8164.13.00 06/09
05/11/2010 14:14

Test	AC	Time
01 Diagnostic	OK	14:15
02 Room Air	RFI*	14:15
03 Room Air	0.000	14:15

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Simul Ser No = 0000000
Std Sol No = 000000
County = 10 Oper No. = 107501

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
MARGY PEARSON

Remarks:

RFI

Form 106-I8000

80-004188
P. 85/88 KM


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004188
Location = LANG 8164.13.00 06/09
05/11/2010 14:43

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:43
02 Std. Gas	0.077	14:44
03 Room Air	0.000	14:44
04 Std. Gas	0.077	14:44
05 Room Air	0.000	14:45
06 Std. Gas	0.077	14:45
07 Room Air	0.000	14:46

Lot No = 659358
Cyl No = 53
Exp Date = 09/03/2011
County = 10 Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

Cal Check 0.080 AC

Form 106-I8000

80-004188
P. 8/6/88 FM


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004188
Location = LANG 8164.13.00 06/09
05/11/2010 14:46

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:47
02 Std. Gas	0.077	14:48
03 Room Air	0.000	14:48
04 Std. Gas	0.077	14:48
05 Room Air	0.000	14:49
06 Std. Gas	0.077	14:49
07 Room Air	0.000	14:50

Lot No = 659358
Cyl No = 53
Exp Date = 09/03/2011
County = 10 Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

Cal Check 0.080 AC

Form 106-I8000

80-004188
P. 87/88 RK


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004188
Location = LANG 8164.13.00 06/09
05/11/2010 14:51

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:51
02 Std. Gas	0.077	14:52
03 Room Air	0.000	14:52
04 Std. Gas	0.076	14:53
05 Room Air	0.000	14:53
06 Std. Gas	0.077	14:53
07 Room Air	0.000	14:54

Lot No = 659358
Cyl No = 53
Exp Date = 09/03/2011
County = 10 Oper No. = 107501

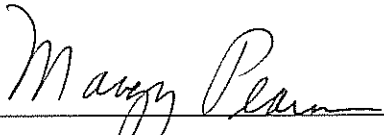

Operator Signature
MARGY PEARSON

Remarks:

Cal Check 0.080 AC

Form 106-I8000

80-004188
P. 88/88 172