

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006498

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 237 psi Regulator: 250 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 20202A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICS 6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 24119080A1 Cyl #: 6 Exp. Date: 11.5.21

Test 1 <u>0.082</u>	Test 4 <u>0.082</u>	Test 7 <u>0.082</u>
Test 2 <u>0.082</u>	Test 5 <u>0.082</u>	Test 8 <u>0.082</u>
Test 3 <u>0.082</u>	Test 6 <u>0.082</u>	Test 9 <u>0.082</u>
Average <u>0.082</u>		

C. Remarks/Maintenance: ANNUAL INSPECTION, REPLACED GAS GAUGE ASSEMBLY, WOULD NOT TAKE TO OPSC., TANK SENSOR CALIBRATION.

Instrument is acceptable to be used in the field.

Charles E. Ehr
Breath Analyst Signature

4.15.21
Date

Kari L. Ditt
Reviewed by

4-19-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006498
Location = TOXL 8164.14.00 09/16
04/15/2021 14:14

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%\$^&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%\$^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 6
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 08/18/2015
Slope 669
Intercept -637469

IR Calibration Date: 08/18/2015

	3um	9um
0th Coef(*100):	-28161	-22508
1st Coef(*100):	286657	143843
2nd Coef(*100):	2341	1281
H2O adj(mg/l*10k):	776	451

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006498
Location = TOXL 8164.14.00 09/16
04/15/2021 14:17

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:18
02 Std. Sol.	0.020	14:18
03 Room Air	0.000	14:19
04 Std. Sol.	0.019	14:20
05 Room Air	0.000	14:20
06 Std. Sol.	0.020	14:21
07 Room Air	0.000	14:21

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

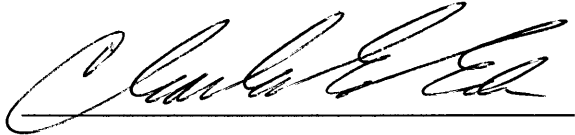

Operator Signature
CHARLES EDER

Remarks: *Low AC*
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006498
Location = TOXL 8164.14.00 09/16
04/15/2021 14:26

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:27
02 Std. Sol.	0.300	14:28
03 Room Air	0.000	14:28
04 Std. Sol.	0.302	14:29
05 Room Air	0.000	14:29
06 Std. Sol.	0.302	14:30
07 Room Air	0.000	14:31

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006498
Location = TOXL 8164.14.00 09/16
04/15/2021 14:40

Test	AC	Time
01 Room Air	0.000	14:41
02 *Subject Test	INT*	14:42
03 Room Air	0.000	14:42

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS921456
Lot No = 24119080A1
Cyl No = 6
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

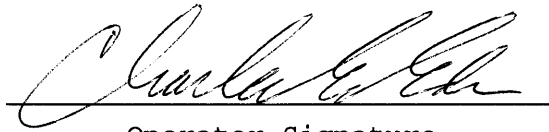

Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006498
Location = TOXL 8164.14.00 09/16
04/15/2021 14:43

Test	AC	Time
01 Diagnostic	OK	14:44
02 Room Air	0.000	14:44
03 *Subject Test	RFI*	14:45
04 Room Air	0.000	14:45

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS921456
Lot No = 24119080A1
Cyl No = 6
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:



Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006498
Location = TOXL 8164.14.00 09/16
04/15/2021 14:46

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:46
02 Std. Gas	0.082	14:47
03 Room Air	0.000	14:47
04 Std. Gas	0.082	14:48
05 Room Air	0.000	14:48
06 Std. Gas	0.082	14:49
07 Room Air	0.000	14:49

Lot No = 24119080A1
Cyl No = 6
Exp Date = 11/05/2021
County = 08 Oper No. = 666666

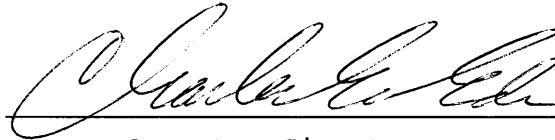

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006498
Location = TOXL 8164.14.00 09/16
04/15/2021 14:53

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:53
02 Std. Gas	0.082	14:54
03 Room Air	0.000	14:54
04 Std. Gas	0.082	14:55
05 Room Air	0.000	14:55
06 Std. Gas	0.082	14:56
07 Room Air	0.000	14:56


Lot No = 24119080A1

Cyl No = 6

Exp Date = 11/05/2021

County = 08

Oper No. = 666666

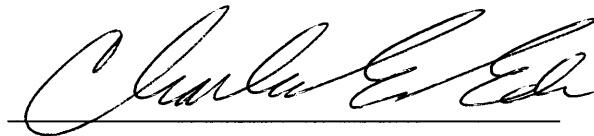

Operator Signature

CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000