

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006490

Location: TBXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 201 psi Regulator: 225 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 2020/2A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICSG Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621080A | Cyl #: 26 Exp. Date: 3.5.23

Test 1	<u>0.078</u>	Test 4	<u>0.078</u>	Test 7	<u>0.080</u>
Test 2	<u>0.079</u>	Test 5	<u>0.078</u>	Test 8	<u>0.079</u>
Test 3	<u>0.079</u>	Test 6	<u>0.079</u>	Test 9	<u>0.079</u>
Average	<u>0.079</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Ehr
Breath Analyst Signature

5/25/21
Date

Kali J. Diet
Reviewed by

5/26/21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006490
Location = TOXL 8164.14.00 09/16
05/25/2021 10:42

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 28
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 09/04/2020
Slope 649
Intercept -598817

IR Calibration Date: 09/04/2020

	3um	9um
0th Coef(*100):	-25190	-16392
1st Coef(*100):	271645	136906
2nd Coef(*100):	2533	1222
H2O adj(mg/l*10k):	460	309

***** Printer Test End *****

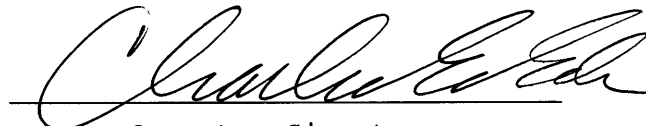
Operator Signature
CHARLES EDER

Remarks: *PRINT TEST*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006490
Location = TOXL 8164.14.00 09/16
05/25/2021 11:15

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:15
02 Std. Sol.	0.018	11:16
03 Room Air	0.000	11:17
04 Std. Sol.	0.019	11:17
05 Room Air	0.000	11:18
06 Std. Sol.	0.019	11:19
07 Room Air	0.000	11:19

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

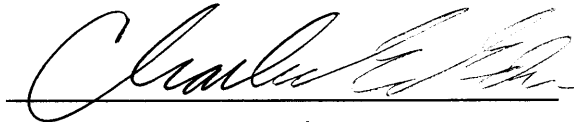

Operator Signature
CHARLES EDER

Remarks: *Low AC*
 0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006490
Location = TOXL 8164.14.00 09/16
05/25/2021 11:26

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:26
02 Std. Sol.	0.304	11:27
03 Room Air	0.000	11:28
04 Std. Sol.	0.303	11:28
05 Room Air	0.000	11:29
06 Std. Sol.	0.303	11:30
07 Room Air	0.000	11:30

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666

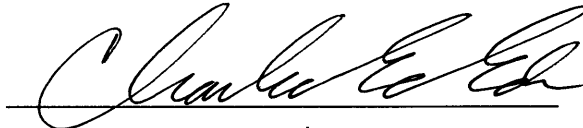

Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006490
Location = TOXL 8164.14.00 09/16
05/25/2021 11:32

Test	AC	Time
01 Room Air	0.000	11:32
02 *Subject Test	INT*	11:33
03 Room Air	0.000	11:33

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS921456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006490
Location = TOXL 8164.14.00 09/16
05/25/2021 11:34

Test	AC	Time
01 Diagnostic	OK	11:34
02 Room Air	0.000	11:35
03 *Subject Test	RFI*	11:35
04 Room Air	0.000	11:36

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS921456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

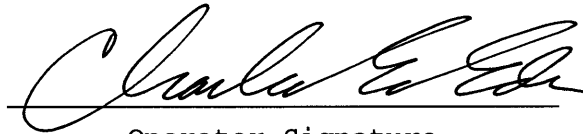

Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006490
Location = TOXL 8164.14.00 09/16
05/25/2021 11:38

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:38
02 Std. Gas	0.078	11:39
03 Room Air	0.000	11:39
04 Std. Gas	0.079	11:40
05 Room Air	0.000	11:40
06 Std. Gas	0.079	11:41
07 Room Air	0.000	11:41

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006490
Location = TOXL 8164.14.00 09/16
05/25/2021 11:42

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:42
02 Std. Gas	0.078	11:42
03 Room Air	0.000	11:43
04 Std. Gas	0.078	11:43
05 Room Air	0.000	11:44
06 Std. Gas	0.079	11:44
07 Room Air	0.000	11:45

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006490
Location = TOXL 8164.14.00 09/16
05/25/2021 11:45

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:46
02 Std. Gas	0.080	11:46
03 Room Air	0.000	11:47
04 Std. Gas	0.079	11:47
05 Room Air	0.000	11:48
06 Std. Gas	0.079	11:48
07 Room Air	0.000	11:49

Lot No = 02621080A1

Cyl No = 26

Exp Date = 03/05/2023

County = 08

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000