



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Jamie M Huschka</u>		
Location: <u>Williams Co. LEC</u>		
Intoxilyzer® Serial Number: <u>80-004184</u>		
Gas Lot Number: <u>15410080A1</u>	Gas Cylinder Number: <u>6</u>	Expiration Date: <u>7/1/12</u>
<input checked="" type="checkbox"/> New Cylinder Installed <input type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%) Test 1: 0. <u>80</u> % Test 2: 0. <u>79</u> % Test 3: 0. <u>80</u> %		
(ATTACH TEST RECORD)		

Jamie M Huschka
Chemical Test Operator Signature

7 Jan 2011
Date

Deb Kashur
Reviewed By

28 Jan 2011
Date

80-004184
P. 96 of 97
JMH

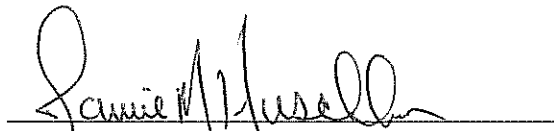
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004184
Location = WILL 8164.13.00 06/09
01/07/2011 13:56

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:57
02 Std. Gas	0.080	13:57
03 Room Air	0.000	13:57
04 Std. Gas	0.079	13:58
05 Room Air	0.000	13:58
06 Std. Gas	0.080	13:59
07 Room Air	0.000	13:59

Lot No = 15410080A1
Cyl No = 6
Exp Date = 07/01/2012
County = 53 Oper No. = 100406


Operator Signature
JAMIE M. HUSCHKA

Remarks:

Form 106-I8000

80-004184
P. 97 of 97
FM