



ETHANOL BREATH STANDARD CYLINDER REPORT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Joe Knowski</u>		
Location: <u>Devils lake LEC</u>		
Intoxilyzer® Serial Number: <u>80-004193</u>		
Gas Lot Number: <u>15410080A1</u>	Gas Cylinder Number: <u>17</u>	Expiration Date: <u>7-1-12</u>
<input checked="" type="checkbox"/> New Cylinder Installed <input type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>074</u> % <u>074</u>		
Test 2: 0. <u>078</u> %		
Test 3: 0. <u>071</u> %		
(ATTACH TEST RECORD)		

Joe Knowski
 Chemical Test Operator Signature

Deb Kashur
 Reviewed By

1-9-2011.
 Date

24 Mar 2011
 Date

80-004193
 p. 91 of 92
 YFM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = DEVL 8164.13.00 06/09
01/09/2011 21:46

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	21:47
02 Std. Gas	0.079	21:47
03 Room Air	0.000	21:48
04 Std. Gas	0.078	21:48
05 Room Air	0.000	21:49
06 Std. Gas	0.079	21:49
07 Room Air	0.000	21:50

DK per Joe Knowski

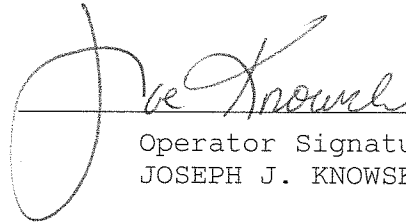
Lot No = ~~659358~~

Cyl No = ~~20~~ 17

Exp Date = ~~09/03/2011~~ 07/01/2012

County = 36

Oper No. = 109208


Operator Signature
JOSEPH J. KNOWSKI

Remarks:

Form 106-I8000

80-004193
p. 92 of 92
JAM