

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program

Form: BrF-105-G

ETHANOL BREATH STANDARD CYLINDER REPORT

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: David J. Zeis

Location: Cavalier County Sheriff's Office Langdon ND

Intoxilyzer Serial No.: 80-004188

Lot Number: 659358

Cylinder Number: 53

Expiration Date: 09/03/11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 080 %

Test 2: 0. 079 %

Test 3: 0. 080 %

(ATTACH TEST RECORD)

David J. Zeis
Chemical Test Operator Signature

02/01/10
Date

Deb Kashner (ACA check)
Reviewed By

02 Feb 2010
Date

80-004188
P. 1 of 2
AK

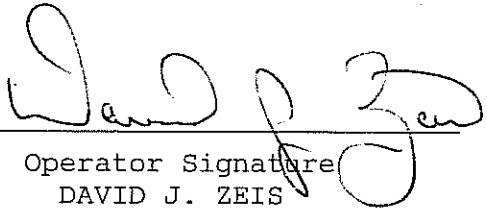
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004188
Location = LANG 8164.13.00 06/09
02/01/2010 13:46

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:47
02 Std. Gas	0.080	13:47
03 Room Air	0.000	13:48
04 Std. Gas	0.079	13:48
05 Room Air	0.000	13:49
06 Std. Gas	0.080	13:49
07 Room Air	0.000	13:50

Lot No = 659358
Cyl No = 53
Exp Date = 09/03/2011
County = 10 Oper No. = 067518


Operator Signature
DAVID J. ZEIS

Remarks:

Form 106-18000

80-004188
P. 2 of 2 KM