



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION

Toxicology Section/Breath Alcohol Program

SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Chris Pulver</u>		
Location: <u>New Town PD</u>		
Intoxilyzer® Serial Number: <u>80-004951</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>36</u>	Expiration Date: <u>12-23-11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%) Test 1: 0. <u>079</u> % Test 2: 0. <u>078</u> % Test 3: 0. <u>079</u> % (ATTACH TEST RECORD)		

Chris Pulver
Chemical Test Operator Signature

2-28-11
Date

Deb Kashner
Reviewed By

01 Mar 2011
Date

80-004951
P. 59 of 60
PM


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004951
Location = NEWT 8164.13.00 06/09
03/03/2011 10:17

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:18
02 Std. Gas	0.079	10:18
03 Room Air	0.000	10:19
04 Std. Gas	0.078	10:19
05 Room Air	0.000	10:20
06 Std. Gas	0.079	10:20
07 Room Air	0.000	10:21

Lot No = 709352
Cyl No = 36
Exp Date = 12/23/2011
County = 31 Oper No. = 049912

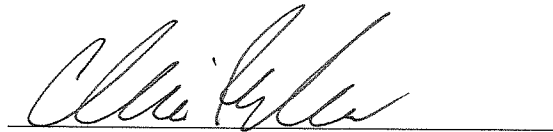

Operator Signature
CHRISTOPHER PULVER

Remarks:

Form 106-I8000

80-004951
P. 60460
pm