



# ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION

Toxicology Section/Breath Alcohol Program

SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Jamie Mituschka</u>		
Location: <u>New Town</u>		
Intoxilyzer® Serial Number: <u>80-004951</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>36</u>	Expiration Date: <u>12/23/2011</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%) Test 1: 0. <u>078</u> % Test 2: 0. <u>077</u> % Test 3: 0. <u>076</u> % <div style="text-align: right;">(ATTACH TEST RECORD)</div>		

Jamie Mituschka  
Chemical Test Operator Signature

23 July 2010  
Date

Deb Kashur  
Reviewed By

24 July 2010  
Date

80-004951  
P. 47 of 48  
VM

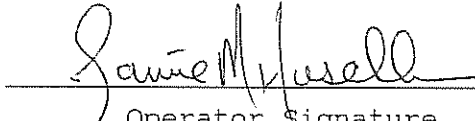
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004951  
Location = NEWT      8164.13.00 06/09  
07/23/2010      09:30

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:32
02 Std. Gas	0.078	09:32
03 Room Air	0.000	09:32
04 Std. Gas	0.077	09:33
05 Room Air	0.000	09:33
06 Std. Gas	0.076	09:34
07 Room Air	0.000	09:34

Lot No = 709352  
Cyl No = 36  
Exp Date = 12/23/2011  
County = 31      Oper No. = 100406

  
Operator Signature  
JAMIE M. HUSCHKA

Remarks:

Form 106-I8000

80-004951  
P. 48 of 48  
JMH