



**ETHANOL BREATH STANDARD CYLINDER REPORT**  
OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Chris Pulver</u>		
Location: <u>New Town PD</u>		
Intoxilyzer® Serial Number: <u>80-004951</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>36</u>	Expiration Date: <u>12-23-11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%) Test 1: 0. <u>079</u> % Test 2: 0. <u>078</u> % Test 3: 0. <u>078</u> % <div style="text-align: right;">(ATTACH TEST RECORD)</div>		

Chris Pulver  
Chemical Test Operator Signature

10-16-10  
Date

Deb Kashner  
Reviewed By

21 Oct 2010  
Date


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004951  
Location = NEWT      8164.13.00 06/09  
10/16/2010      21:27

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	21:28
02 Std. Gas	0.079	21:29
03 Room Air	0.000	21:29
04 Std. Gas	0.078	21:29
05 Room Air	0.000	21:30
06 Std. Gas	0.078	21:30
07 Room Air	0.000	21:31

Lot No = 709352  
Cyl No = 36  
Exp Date = 12/23/2011  
County = 31      Oper No. = 049912

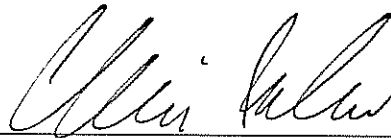

Operator Signature  
CHRISTOPHER PULVER

Remarks:

Form 106-I8000

80-004951  
P. 59 of 54  
km