



**ETHANOL BREATH STANDARD CYLINDER REPORT**  
 OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION  
 Toxicology Section/Breath Alcohol Program  
 SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Joe Krawski</u>		
Location: <u>Devils lake LEC.</u>		
Intoxilyzer® Serial Number: <u>80-004193</u>		
Gas Lot Number: <u>659358</u>	Gas Cylinder Number: <u>20</u>	Expiration Date: <u>9-3-2011</u>
<input type="checkbox"/> New Cylinder Installed	<input type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: <u>0.081</u> %		
Test 2: <u>0.081</u> %		
Test 3: <u>0.080</u> %		
(ATTACH TEST RECORD)		

Joe Krawski  
 Chemical Test Operator Signature

11-11-2010  
 Date

Deb Kashur  
 Reviewed By

10-Jan-2011  
 Date

80-004193  
 P. 87 of 88  
 JAH

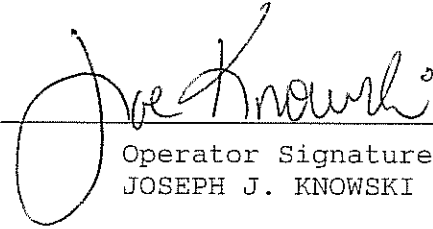
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004193  
Location = DEVL      8164.13.00 06/09  
11/11/2010      20:14

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	20:15
02 Std. Gas	0.081	20:15
03 Room Air	0.000	20:16
04 Std. Gas	0.081	20:16
05 Room Air	0.000	20:17
06 Std. Gas	0.080	20:17
07 Room Air	0.000	20:18

Lot No = 659358  
Cyl No = 20  
Exp Date = 09/03/2011  
County = 36      Oper No. = 109208

  
Operator Signature  
JOSEPH J. KNOWSKI

Remarks:

Form 106-I8000

80-004193  
P. 88 of 88  
FM