

ETHANOL BREATH STANDARD CYLINDER REPORT

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Richard D. Johnson

Location: McLean S.O. Washburn

Intoxilyzer Serial No.: 80-004196

Lot Number: ~~6~~ 659357

Cylinder Number: 47

Expiration Date: 9-3-11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0.081 %

Test 2: 0.081 %

Test 3: 0.082 %

(ATTACH TEST RECORD)

Richard Johnson
Chemical Test Operator Signature

11-24-09
Date

Deb Kashner
Reviewed By

04 Dec 09
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = WASH 8164.13.00 06/09
11/24/2009 14:20

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:21
02 Std. Gas	0.081	14:21
03 Room Air	0.000	14:22
04 Std. Gas	0.081	14:22
05 Room Air	0.000	14:23
06 Std. Gas	0.082	14:23
07 Room Air	0.000	14:23

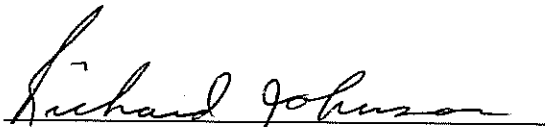
Lot No = 659357

Cyl No = 47

Exp Date = 09/03/2011

County = 28

Oper No. = 118707


Operator Signature
RICHARD D. JOHNSON

Remarks:

Form 106-I8000

80-004196
P. 2 of 2 JH