

**INTOXILYZER® 8000 INITIAL INSPECTION**

Intoxilyzer® 8000 Serial Number: 80-006491

**1) GENERAL Setup and Checks:**

- a)  Power On
  - 5 min. countdown during initial warm-up
  - 1 min. countdown to begin test after standby mode
- b)  Display Intensity (Ctrl + ↑ or ↓)
- c) Password Security:
  - Level 1 (Operator)     Level 2 (Field Inspector)     Level 3 (Lab Personnel)
- d)  Printer Setup (Level 3,S,P)
- e)  Forms Load (CMI, Inc., CoBrA Software)

**2) LEVEL 1 Setup and Checks:**

- a)  Internal Printer Test and Paper Feed (Level 1,P). Attach record.
- b)  External Printer Test (Level 1,P). Attach record.
- c) Barcode Reader (Level 1,B):
  - Operator ID     ND License     R key: Refusal. Attach record.

**3) LEVEL 2 Setup and Checks:**

- a)  Continuous Air Blank (Level 2,A)
- b)  Diagnostic (Level 2,D). Attach record.
- c)  Prelim Data Entry (Level 2,E)
- d) Ser Number/Version Info (Level 2,V):
  - Inst Ser#: 80-006491    DSP Ver: 1362.14
  - Core Ver: 8164.13    CPLD Ver: 7

**4) LEVEL 3 Setup and Checks:**

- a) DVM Monitor (Level 3,D,D): 3: 12447 s: 1 C: 47.00  
9: 13006 s: 2 B: 45 0  
(RFI indicator with keyed radio): 1
- b) Function (F) Keys :  F5 – Tone                       F9 - Fan  
 F6 – Green LED                     F10 – Pump  
 F7 – Red LED                         F11 – Solenoid
- c) Atmospheric Monitor (Level 3,D,A): Atmo Sensor, P: 950 CF: 1.06
- d) Flow Monitor (Level 3,D,F): Flow Sensor, R: 205 F: 0.000 L/s

- e) Temperature Monitor (Level 3,D,T): C: 47.0 A: 45.0 I: 0.0  
B: 45.1 V: 0.0 <sup>~1000</sup>
- f) Tank Monitor (Level 3,D,G): P (display): 1001 psi P (gauge): 7000 psi  
<sub>000</sub>
- g)  General Setup (Level 3,S,G)
- h)  Configure Start Test (Level 3,S,T)
- i)  Network (Level 3,S,N)

**5) TESTS (attach all test records):**

**Configure wet bath simulator standards before running tests (Level 1,S):**

- a) Zero AC (Level 1,C):  
Sim ser #: MP3067 Lot #: MILLIQ H<sub>2</sub>O Exp date: NA  
Known value: 0.000  
Results: 0.000 AC 0.000 AC 0.000 AC
- b) Low AC (Level 1,C):  
Sim ser #: MP3066 Lot #: 15160 Exp date: 7/14/17  
Known value: 0.020  
Results: 0.020 AC 0.019 AC 0.019 AC
- c) High AC (Level 1,C):  
Sim ser #: MP3068 Lot #: 14102 Exp date: 4/23/16  
Known value: 0.400  
Results: 0.397 AC 0.399 AC 0.399 AC

**Configure dry gas standard before running tests (Level 1,S):**

- d) Ethanol + 0.05% Acetone (Level 1,B):  
Sim ser #: DR5135 Lot #: ICS4 Exp date: 9/9/2017  
Known value: 0.10 AC + 0.05% ACETONE  
 Display reads "Interferent Detect"
- e) Acetone (Level 1,B):  
Sim ser #: DR5143 Lot #: ACE2 Exp date: 9/29/2017  
Known value: 0.05% ACETONE  
 Display reads "Interferent Detect"
- f) Methanol (Level 1,B):  
Sim ser #: PR3377 Lot #: MET2 Exp date: 9/29/2017  
Known value: 0.10% METHANOL  
 Display reads "Interferent Detect"
- g) Isopropanol (Level 1,B):  
Sim ser #: DR3453 Lot #: IPA2 Exp date: 9/29/2017  
Known value: 0.10% ISOPROPRANOL  
 Display reads "Interferent Detect"

- h)  Ambient Fail (Level 1,B): Display and test record read correct.
- i)  Invalid Sample (Level 1,B): Display and test record read correct.
- j)  Sequence Aborted (Level 1,B): Display and test record read correct.
- k)  ABA (Level 1,B): Test record reads correct.
- l)  Calibration Check Out of Tolerance (CMS mode): Display and test record read correct.
- m)  RFI Detected (B,C, or CMS mode): Display and test record read correct.
- n)  Tank Pressure Below Minimum (CMS mode): Display reads correct.
- o)  Deficient Samples (CMS mode): Display and test record read correct.
- p)  Improper Sample (CMS mode): Display and test record read correct.
- q)  Difference Too Great (CMS mode): Display and test record read correct.
- r)  CMS (CMS mode): Test record reads correct.
- s) Stability Test (Level 3,T,S):

Ave: 0.0811 Std Dev: 0.0006 Rel Std Dev: 0.75%

Maintenance/Repairs/Notes: \_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

Instrument is acceptable to be used in the field.

Charles E. Edner  
Field Inspector's Signature

1/19/16  
Date

Deb Shanaver  
Reviewed by

19 Jan 16  
Date

Intoxilyzer Test Record and Checklist  
NDDAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer  
North Dakota Model 8000 SN 80-006491  
Location ~~CMI~~ 8164.13.00 06/09  
01/15/2016 *ToxL* 16:04  
*CEC*

\*\*\*\*\* Printer Test \*\*\*\*\*

12 char/line  
abcdefghijkl  
ABCDEFGHIJKL

16 char per line  
abcdefghijklmnop  
ABCDEFGHIJKLMN

21 chars per line  
abcdefghijklmnopqrstu  
ABCDEFGHIJKLMN

24 characters per line  
abcdefghijklmnopqrstu  
ABCDEFGHIJKLMN

32 characters per line  
abcdefghijklmnopqrstu  
ABCDEFGHIJKLMN

42 characters per line  
abcdefghijklmnopqrstu  
ABCDEFGHIJKLMN

Current Instrument Status

Data Entry Mode: *Special*  
Start Test Sequence: DABACABH  
Display Prelim Rslt? Yes  
Display Third Digit? Yes  
Inhib Printer(Y/N)? No  
Display Volume? No  
Disable On MemFull? No  
# of Print Copies? 1  
Select Std (D/W/I)? Dry  
Standard Value? 0.080  
Standard Lot #? 123  
Standard Cyl #? 12345  
Standard Expiration? 11/11/2020  
Oper No? 666666

Flow Cal. Date: 08/18/2015  
Slope: 669  
Intercept: -662544

IR Calibration Date: 08/18/2015  
3um 9um

0th Coef(\*100): -27273 -22751  
1st Coef(\*100): 272579 140235  
2nd Coef(\*100): 1982 1330  
H2O adj(mg/l)\*10k: 664 431

\*\*\*\*\* Test End \*\*\*\*\*



Operator Signature  
CHARLES EDER

Remarks: *PRINT TEST*

Form 106-18000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006491  
Location = ~~CMI~~ <sup>CEE</sup>            8164.13.00 06/09  
01/15/2016            <sup>TOXL</sup>            16:08

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^&\*()\_+?

Current Instrument Setup

Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        No  
# of Print Copies?          1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            19615080A5  
Standard Cyl #?            3  
Standard Expiration?        09/05/2017  
Oper No?                    666666

Flow Cal. Date:            08/18/2015  
Slope                        669  
Intercept                    -662544

IR Calibration Date:        08/18/2015  
                                  3um                    9um

-----  
0th Coef(\*100):            -27273                    -22751  
1st Coef(\*100):            272579                    140235  
2nd Coef(\*100):            1982                      1330  
H2O adj(mg/l\*10k):        664                        431

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
CHARLES EDER

Remarks:

PRINT TEST

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer                      Alcohol Analyzer  
North Dakota Model 8000                      SN 80-006491  
Location = ~~CMI~~ <sup>CEC</sup>                      8164.13.00 06/09  
01/15/2016                      <sup>TOXL</sup>                      16:09

Test	AC	Time
01 Room Air	0.000	16:10
02 *Subject Test	REF*	16:10
03 Room Air	0.000	16:10

\*Subject Test Refused

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                      Weight = 150  
Test = DUI                      Cit = REFUSAL  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08                      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

REFUSAL

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = *CMI TOXL*      8164.13.00 06/09  
01/15/2016 *CEE*      16:22

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *DIAGNOSTIC*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/15/2016      16:30

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:31
02 Std. Sol.	0.000	16:32
03 Room Air	0.000	16:32
04 Std. Sol.	0.000	16:33
05 Room Air	0.000	16:34
06 Std. Sol.	0.000	16:34
07 Room Air	0.000	16:35

08 Sim Temp = 34.0°C

Simul Ser No = MP3067  
Std Sol No = MILLIQ H2O  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

ZERO AC  
0.000 AC

Form 106-I8000



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/15/2016      16:37

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:38
02 Std. Sol.	0.020	16:39
03 Room Air	0.000	16:39
04 Std. Sol.	0.019	16:40
05 Room Air	0.000	16:40
06 Std. Sol.	0.019	16:41
07 Room Air	0.000	16:42

08 Sim Temp = 34.0°C

Simul Ser No = MP3066  
Std Sol No = 15160  
County = 08      Oper No. = 666666

  
\_\_\_\_\_  
Operator Signature  
CHARLES EDER

Remarks:      *Low AC*  
                    *0.020 AC*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/15/2016      16:44

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:44
02 Std. Sol.	0.397	16:45
03 Room Air	0.000	16:46
04 Std. Sol.	0.399	16:46
05 Room Air	0.000	16:47
06 Std. Sol.	0.399	16:48
07 Room Air	0.000	16:48

08 Sim Temp = 34.0°C

Simul Ser No = MP3068  
Std Sol No = 14102  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

HIGH AC  
0.400 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006491  
Location = TOXL                    8164.13.00 06/09  
01/19/2016                            10:05

Test	AC	Time
01 Room Air	0.000	10:07
02 *Subject Test	INT*	10:07
03 Room Air	0.000	10:08

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = 0.10AC+0.05ACE  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*INTERFERENT DETECT*  
*0.10AC + 0.05% ACETONE*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006491  
Location = TOXL                8164.13.00 06/09  
01/19/2016                        10:21

Test	AC	Time
01 Room Air	0.000	10:22
02 *Subject Test	INT*	10:23
03 Room Air	0.000	10:23

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                Weight = 150  
Test = DUI                        Cit = 0.05 ACETONE  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08                        Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *INTERFERENT DETECT*  
*0.05% ACETONE*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/19/2016      10:24

Test	AC	Time
01 Room Air	0.000	10:24
02 *Subject Test	INT*	10:25
03 Room Air	0.000	10:26

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = 0.10 METHANOL  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08      Oper No. = 666666

  
\_\_\_\_\_  
Operator Signature  
CHARLES EDER

Remarks: *INTERFERENT DETECT*  
*0.10% METHANOL*


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/19/2016      10:27

Test	AC	Time
01 Room Air	0.000	10:28
02 *Subject Test	INT*	10:28
03 Room Air	0.000	10:29

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = 0.10 IPA  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *INTERFERENT DETECT*  
*0.10% ISOPROPAVOL*


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/19/2016      11:00

Test	AC	Time
01 Room Air	AMB*	11:01
02 Room Air	0.000	11:02

\*Invalid Test  
Check Ambient Conditions

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = AMBIENT FAIL  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08      Oper No. = 666666

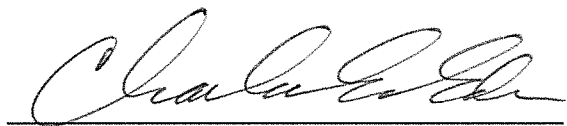

Operator Signature  
CHARLES EDER

Remarks:

*AMBIENT FAIL*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/19/2016      11:03

Test	AC	Time
01 Room Air	0.000	11:04
02 Invalid Sample	X.XXX	11:04
03 Room Air	0.000	11:05

\*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = INVALID SAMPLE  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *INVALID SAMPLE*



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/19/2016      11:05

Test	AC	Time
01 Room Air	0.000	11:06
02 *Subject Test	ABT*	11:06
03 Room Air	0.000	11:07

\*Sequence Aborted

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = SEQ ABORTED  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: SEQUENCE ABORTED


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/19/2016      11:08

Test	AC	Time
01 Room Air	0.000	11:08
02 Subject Test 1	0.000	11:09
03 Room Air	0.000	11:09
04 Reported AC	0.000	11:09

No RFI Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = ABA TEST  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08      Oper No. = 666666

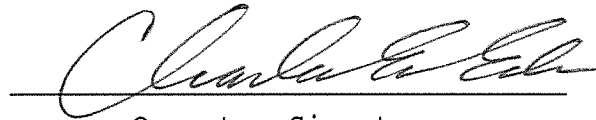

Operator Signature  
CHARLES EDER

Remarks:

ABA TEST

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer  
North Dakota Model 8000 SN 80-006491  
Location = TOXL 8164.13.00 06/09  
01/19/2016 11:10

Test	AC	Time
01 Diagnostic	OK	11:11
02 Room Air	0.000	11:12
03 Subject Test 1	0.000	11:12
04 Room Air	0.000	11:17
05 Std. Gas	0.086*	11:18
06 Room Air	0.000	11:18

\*Cal Check Out of Tolerance

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female Weight = 150  
Test = DUI Cit = CAL OUT OF TOL  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

CALIBRATION CHECK  
OUT OF TOLERANCE

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/19/2016      11:20

Test	AC	Time
01 Diagnostic	OK	11:20
02 Room Air	0.000	11:21
03 *Subject Test	RFI*	11:21
04 Room Air	0.000	11:22

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = RFI  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08      Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

RFI DETECT

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/19/2016      11:23

Test	AC	Time
01 Diagnostic	OK	11:24
02 Room Air	0.000	11:24
03 *Subject Test	0.000*	11:27
04 Room Air	0.000	11:33
05 Std. Gas	0.081	11:34
06 Room Air	0.000	11:35
07 *Subject Test	0.000*	11:38
08 Room Air	0.000	11:39


No RFI Detected

\*Deficient Sample - Value Printed was  
Highest Obtained

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = DEFICIENT SAMP  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08      Oper No. = 666666

20 minute waiting period ascertained? Y  
Clean Mouthpiece used and disposed? Y  
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the  
instructions displayed by the Intoxilyzer  
in conducting this test.

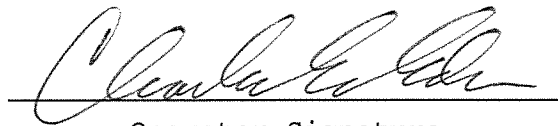

Operator Signature  
CHARLES EDER

Remarks: DEFICIENT SAMPLES

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/19/2016      11:40

Test	AC	Time
01 Diagnostic	OK	11:41
02 Room Air	IPS*	11:41
03 Room Air	0.000	11:41

\*Improper Sample

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = IMPROPER SAMPLE  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08      Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

*IMPROPER SAMPLE*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/19/2016      11:42

Test	AC	Time
01 Diagnostic	OK	11:43
02 Room Air	0.000	11:44
03 Subject Test 1	0.144*	11:44
04 Room Air	0.000	11:47
05 Std. Gas	0.081	11:48
06 Room Air	0.000	11:49
07 Subject Test 2	0.198*	11:50
08 Room Air	0.000	11:51

\*Difference Too Great

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = DIFF TOO GREAT  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08      Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

DIFFERENCE  
Too GREAT

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006491  
Location = TOXL                    8164.13.00 06/09  
01/19/2016                            11:52

Test	AC	Time
01 Diagnostic	OK	11:53
02 Room Air	0.000	11:54
03 Subject Test 1	0.194	11:54
04 Room Air	0.000	11:57
05 Std. Gas	0.078	11:58
06 Room Air	0.000	11:59
07 Subject Test 2	0.195	12:00
08 Room Air	0.000	12:01
09 Reported AC	0.194	11:54

Difference OK  
No RFI Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = CMS TEST  
Dr. Lic. = ND/DIS821456  
Lot No = 19615080A5  
Cyl No = 3  
Expiration Date = 09/05/2017  
County = 08                            Oper No. = 666666

20 minute waiting period ascertained? Y  
Clean Mouthpiece used and disposed? Y  
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

CMS TEST



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006491  
Location = TOXL      8164.13.00 06/09  
01/19/2016      12:07

Test	AC	Time
01 Room Air	0.000	12:08
02 Std. Gas	0.082	12:08
03 Room Air	0.000	12:09
04 Std. Gas	0.081	12:09
05 Room Air	0.000	12:09
06 Std. Gas	0.081	12:10
07 Room Air	0.000	12:10
08 Std. Gas	0.081	12:11
09 Room Air	0.000	12:11
10 Std. Gas	0.080	12:12
11 Room Air	0.000	12:12
12 Std. Gas	0.081	12:13
13 Room Air	0.000	12:13
14 Std. Gas	0.081	12:14
15 Room Air	0.000	12:14
16 Std. Gas	0.081	12:15
17 Room Air	0.000	12:15
18 Std. Gas	0.080	12:15
19 Room Air	0.000	12:16
20 Std. Gas	0.080	12:16
21 Room Air	0.000	12:17
22 Std. Gas	0.082	12:17
23 Room Air	0.000	12:18
24 Std. Gas	0.082	12:18
25 Room Air	0.000	12:19
26 Std. Gas	0.081	12:19
27 Room Air	0.000	12:20
28 Std. Gas	0.081	12:20
29 Room Air	0.000	12:21
30 Std. Gas	0.081	12:21
31 Room Air	0.000	12:22
32 Std. Gas	0.081	12:22
33 Room Air	0.000	12:23
34 Std. Gas	0.082	12:23
35 Room Air	0.000	12:24
36 Std. Gas	0.081	12:24
37 Room Air	0.000	12:25
38 Std. Gas	0.081	12:25
39 Room Air	0.000	12:25
40 Std. Gas	0.081	12:26
41 Room Air	0.000	12:26
42 Cal Check Stats:		
43 Average	0.0811	
44 Std Dev	0.0006	
45 Rel Std Dev	0.75%	

*Charles E. Eder*  
STABILITY TEST

Operator Signature  
CHARLES EDER

Remarks:

STABILITY TEST

Form 106-I8000

*Charles Eder*  
1/19/16

LOT: 1961508045

Exp: 9/5/2017

CYL: 003