

**CHAIN OF CUSTODY
BREATH ALCOHOL INSTRUMENT**

Instrument: 8000 Serial Number: 80-007094

Agency being assigned instrument: DUMP (DISPOSED OF)

Date 8/5/2021

Transferred from:

Transferred to:

Name (print) CHARLES E. EDER

Name (print) DUMP (DISPOSED)

Signature *Charles E. Eder*

Signature _____

Agency O.A.G. - CRIME LAB

Agency DUMP (DISPOSED)

Reason for transfer/remarks:

- EEPROM ERROR, SYSTEM FAULT ID#18
- FACTORY REPAIR IS COST PROHIBITIVE
- COMPONENTS WILL BE SAVED FOR REPAIRS AND MAINTENANCE OF OTHER UNITS.

Or Shipped Via:

USPS _____ UPS _____ FedEx _____ Other _____

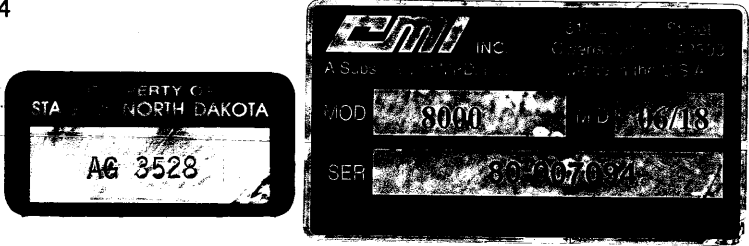
Date Sending Instrument: _____ / _____ / _____ Air Bill No. _____



PROPERTY DISPOSAL
OFFICE OF ATTORNEY GENERAL
 SFN 60567 (12/2020)

Multiple quantities of like items may be listed on one form and attach a sheet with tag numbers and serial numbers if available. Use a separate form for different items.


Division Crime Laboratory	Location of Property Breath Lab - Room 148	Date 8/5/21
Point of Contact Charles E. Eder	Point of Contact Email ceder@nd.gov	Point of Contact Telephone Number 7013286156

Description of Property (make, model, color, etc.) Intoxilyzer 8000 Evidential Breath Alcohol Analyzer - CMI, Inc., Owensboro, KY Unit 80-007094 	Tag Number (if available) AG 3528
	Serial Number (if available) 80-007094
	Date Purchased (if available)
	Original Cost (if available)

Reason for disposal
 EEPROM Fault, System Fault ID #018 - This fault is cost prohibitive as a factory repair. Appropriate components will be kept for normal maintenance and repairs of other units.

Method of disposal:

- Landfill
- Trash can/dumpster
- Electronics Disposal

Signature of person disposing property 
Date 8/5/2021

Send form to Tasha Gerding, Finance Division

Authorized Representative Signature
Date