

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-007098 Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 936 psi Regulator: 950 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICS6 Exp. Date: NA

Display reads "Interferent Detect"

3. RFI Check (CMS Mode) Display reads "RFI Detect"

4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC

Gas Cyl Lot #: 02621080A1 Cyl #: 25 Exp. Date: 3.5.23

Test 1 0.081 Test 4 0.082 Test 7 0.080

Test 2 0.082 Test 5 0.081 Test 8 0.081

Test 3 0.080 Test 6 0.081 Test 9 0.081

Average 0.081

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Breath Analyst Signature

Reviewed by

5.7.21
Date

5-10-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007098
Location = TOXL 8164.16.00 09/18
05/07/2021 14:16

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 2
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 09/26/2018
Slope 684
Intercept -588446

IR Calibration Date: 09/26/2018

	3um	9um
0th Coef(*100):	-40948	-15551
1st Coef(*100):	237555	134140
2nd Coef(*100):	2571	1433
H2O adj(mg/l*10k):	1097	457

***** Printer Test End *****

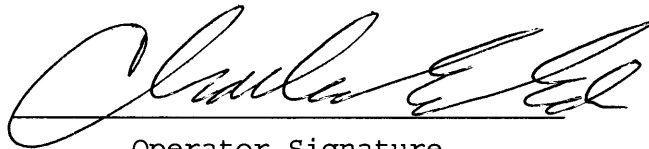

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007098
Location = TOXL 8164.16.00 09/18
05/07/2021 14:25

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:25
02 Std. Sol.	0.019	14:26
03 Room Air	0.000	14:27
04 Std. Sol.	0.020	14:28
05 Room Air	0.000	14:28
06 Std. Sol.	0.020	14:29
07 Room Air	0.000	14:29

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Low AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007098
Location = TOXL 8164.16.00 09/18
05/07/2021 14:34

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:34
02 Std. Sol.	0.301	14:35
03 Room Air	0.000	14:36
04 Std. Sol.	0.303	14:36
05 Room Air	0.000	14:37
06 Std. Sol.	0.300	14:38
07 Room Air	0.000	14:38

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007098
Location = TOXL 8164.16.00 09/18
05/07/2021 14:39

Test	AC	Time
01 Room Air	0.000	14:40
02 *Subject Test	INT*	14:41
03 Room Air	0.000	14:41

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

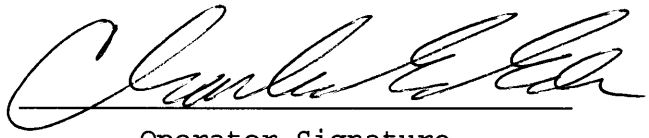

Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10 AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007098
Location = TOXL 8164.16.00 09/18
05/07/2021 14:42

Test	AC	Time
01 Diagnostic	OK	14:42
02 Room Air	0.000	14:43
03 *Subject Test	RFI*	14:43
04 Room Air	0.000	14:43

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

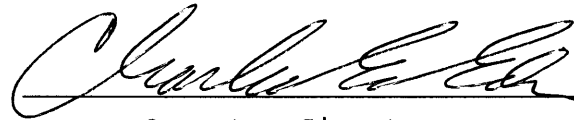

Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007098
Location = TOXL 8164.16.00 09/18
05/07/2021 14:44

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:45
02 Std. Gas	0.081	14:45
03 Room Air	0.000	14:46
04 Std. Gas	0.082	14:46
05 Room Air	0.000	14:47
06 Std. Gas	0.080	14:47
07 Room Air	0.000	14:47

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

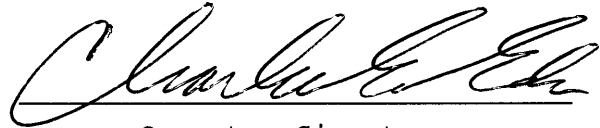

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007098
Location = TOXL 8164.16.00 09/18
05/07/2021 14:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:48
02 Std. Gas	0.082	14:49
03 Room Air	0.000	14:49
04 Std. Gas	0.081	14:50
05 Room Air	0.000	14:50
06 Std. Gas	0.081	14:50
07 Room Air	0.000	14:51


Lot No = 02621080A1

Cyl No = 25

Exp Date = 03/05/2023

County = 08

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007098
Location = TOXL 8164.16.00 09/18
05/07/2021 14:51

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:52
02 Std. Gas	0.080	14:52
03 Room Air	0.000	14:53
04 Std. Gas	0.081	14:53
05 Room Air	0.000	14:54
06 Std. Gas	0.081	14:54
07 Room Air	0.000	14:54

Lot No = 02621080A1

Cyl No = 25

Exp Date = 03/05/2023

County = 08

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000