

INTOXILYZER® 8000 INITIAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-007092

A. GENERAL Setup and Checks:

- 1. Power On
 - 5 min. countdown during initial warm-up
 - 1 min. countdown to begin test after standby mode
- 2. Display Intensity (Ctrl + ↑ or ↓)
- 3. Password Security:
 - Level 1 (Operator) Level 2 (Field Inspector) Level 3 (Lab Personnel)
- 4. Printer Setup (Level 3,S,P)
- 5. Forms Load (CMI, Inc., CoBrA Software)

B. LEVEL 1 Setup and Checks:

- 1. Internal Printer Test and Paper Feed (Level 1,P). Attach record.
- 2. External Printer Test (Level 1,P). Attach record.
- 3. Barcode Reader (Level 1,B):
 - Operator ID ND License R key: Refusal. Attach record.

C. LEVEL 2 Setup and Checks:

- 1. Continuous Air Blank (Level 2,A)
- 2. Diagnostic (Level 2,D). Attach record.
- 3. Prelim Data Entry (Level 2,E)
- 4. Ser Number/Version Info (Level 2,V):
 - Inst Ser#: 80-007092 DSP Ver: 1362.14
 - Core Ver: 8164.16 CPLD Ver: 7

D. LEVEL 3 Setup and Checks:

- 1. DVM Monitor (Level 3,D,D): 3: 12641 s: 2 C: 47.00
9: 13274 s: 2 B: 45 0
(RFI indicator with keyed radio): 1
- 2. Function (F) Keys: : F5 – Tone F9 - Fan
 F6 – Green LED F10 – Pump
 F7 – Red LED F11 – Solenoid
- 3. Atmospheric Monitor (Level 3,D,A): Atmo Sensor, P: 957 CF: 1.05
- 4. Flow Monitor (Level 3,D,F): Flow Sensor, R: 187 F: 0.000 L/s

5. Temperature Monitor (Level 3,D,T): C: 47.0 A: 48.5 I: 0.0
B: 45.1 V: 0.0
6. Tank Monitor (Level 3,D,G): P (display): 652 psi P (gauge): 650 psi
7. General Setup (Level 3,S,G)
8. Configure Start Test (Level 3,S,T)
9. Network (Level 3,S,N)

E. TESTS (attach all test records):

Configure wet bath simulator standards before running tests (Level 1,S):

1. Zero AC (Level 1,C):
Sim ser #: DR3377 Lot #: MILLI OH₂O Exp date: NA
Known value: 0.000 AC
Results: 0.000 AC 0.000 AC 0.000 AC
2. Low AC (Level 1,C):
Sim ser #: DR7111 Lot #: 17160 Exp date: 6.8.19
Known value: 0.020 AC
Results: 0.019 AC 0.019 AC 0.020 AC
3. High AC (Level 1,C):
Sim ser #: DR5186 Lot #: 17010 Exp date: 5/2/2019
Known value: 0.250 AC
Results: 0.245 AC 0.245 AC 0.244 AC

Configure dry gas standard before running tests (Level 1,S):

4. Ethanol + 0.05% Acetone (Level 1,B):
Sim ser #: DR7089 Lot #: ICS #5 Exp date: 5.15.19
Known value: 0.10AC + 0.05% ACETONE
 Display reads "Interferent Detect"
5. Acetone (Level 1,B):
Sim ser #: DR3846 Lot #: ACE 1 Exp date: NA
Known value: 0.05% ACETONE
 Display reads "Interferent Detect"
6. Methanol (Level 1,B):
Sim ser #: DR3455 Lot #: MET 2 Exp date: NA
Known value: 0.10% METHANOL
 Display reads "Interferent Detect"
7. Isopropanol (Level 1,B):
Sim ser #: DR5189 Lot #: IPA 2 Exp date: NA
Known value: 0.10% ISOPROPANOL
 Display reads "Interferent Detect"

- 8. Ambient Fail (Level 1,B): Display and test record read correct.
- 9. Invalid Sample (Level 1,B): Display and test record read correct.
- 10. Sequence Aborted (Level 1,B): Display and test record read correct.
- 11. ABA (Level 1,B): Test record reads correct.
- 12. Calibration Check Out of Tolerance (CMS mode): Display and test record read correct.
- 13. RFI Detected (B,C, or CMS mode): Display and test record read correct.
- 14. Tank Pressure Below Minimum (CMS mode): Display reads correct.
- 15. Deficient Samples (CMS mode): Display and test record read correct.
- 16. Improper Sample (CMS mode): Display and test record read correct.
- 17. Difference Too Great (CMS mode): Display and test record read correct.
- 18. CMS (CMS mode): Test record reads correct.
- 19. Stability Test (Level 3,T,S):

Ave: 0.0804 Std Dev: 0.0005 Rel Std Dev: 0.63%

Maintenance/Repairs/Notes: INITIAL INSPECTION AFTER RECEIVING
FROM CMI, INC.

Instrument is acceptable to be used in the field.

Charles E. Edie

Field Inspector's Signature

10/12/2018
Date

Roberta Huggins-Timmer

Reviewed by

18 Oct 18
Date

Intoxilyzer Test Record and Checklist
NDDAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 11:56

***** Printer Test *****

12 char/line
abcdefghijkl
ABCDEFGHIJKL

16 char per line
abcdefghijklmnop
ABCDEFGHIJKLMN

21 chars per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMN

24 characters per line
abcdefghijklmnopqrstuvwx
ABCDEFGHIJKLMN

32 characters per line
abcdefghijklmnopqrstuvwxy123456
ABCDEFGHIJKLMN

42 characters per line
abcdefghijklmnopqrstuvwxy1234567890abcdef
ABCDEFGHIJKLMN

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DRABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On MenFull? No
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 80
Standard Cyl #? 1111
Standard Expiration? 11/11/2019
Oper No? 666666

Flow Cal. Date: 09/26/2018
Slope 670
Intercept -596123

IR Calibration Date: 09/26/2018

	3um	9um
0th Coef(*100):	-27453	-17291
1st Coef(*100):	248629	134601
2nd Coef(*100):	2770	1393
H2O adj(mg/l*10k):	872	414

***** Test End *****



Operator Signature
CHARLES EDER

Remarks: INTERNAL
PRINT
TEST
Form 106-18000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 11:59

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? No
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 80
Standard Cyl #? 1111
Standard Expiration? 11/11/2019
Oper No? 666666

Flow Cal. Date: 09/26/2018
Slope 670
Intercept -596123

IR Calibration Date: 09/26/2018
 3um 9um

0th Coef(*100): -27453 -17291
1st Coef(*100): 248629 134601
2nd Coef(*100): 2770 1393
H2O adj (mg/l*10k): 872 414

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks: *EXTERNAL PRINT*
TEST


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 12:01

Test	AC	Time
01 Room Air	0.000	12:02
02 *Subject Test	REF*	12:02
03 Room Air	0.000	12:02

*Subject Test Refused

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = R KEY REFUSAL
Dr. Lic. = ND/DIS821456
Lot No = 80
Cyl No = 1111
Expiration Date = 11/11/2019
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: BARCODE READER
 "R" KEY REFUSAL

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 12:04

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

DIAGNOSTIC

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 14:31

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:32
02 Std. Sol.	0.019	14:33
03 Room Air	0.000	14:33
04 Std. Sol.	0.019	14:34
05 Room Air	0.000	14:34
06 Std. Sol.	0.020	14:35
07 Room Air	0.000	14:36

08 Sim Temp = 34.0°C

Simul Ser No = DR7111
Std Sol No = 17160
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Low AC

0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 14:44

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:45
02 Std. Sol.	0.245	14:46
03 Room Air	0.000	14:46
04 Std. Sol.	0.245	14:47
05 Room Air	0.000	14:47
06 Std. Sol.	0.244	14:48
07 Room Air	0.000	14:49

08 Sim Temp = 34.0°C

Simul Ser No = DR5186
Std Sol No = 17010
County = 08 Oper No. = 666666

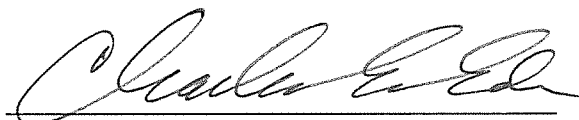

Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.250 AC

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 14:59

Test	AC	Time
01 Room Air	0.000	15:00
02 *Subject Test	INT*	15:01
03 Room Air	0.000	15:01

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10 AC + 0.05% ACETONE


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 15:02

Test	AC	Time
01 Room Air	0.000	15:03
02 *Subject Test	INT*	15:03
03 Room Air	0.000	15:04

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Clock
0.1 0.05% ACETONE
all

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 15:05

Test	AC	Time
01 Room Air	0.000	15:06
02 *Subject Test	INT*	15:06
03 Room Air	0.000	15:07

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10% METHANOL

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 15:07

Test	AC	Time
01 Room Air	0.000	15:08
02 *Subject Test	INT*	15:08
03 Room Air	0.000	15:09

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10% ISOPROPNOL

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 15:49

Test	AC	Time
01 Room Air	AMB*	15:50
02 Room Air	0.000	15:50

*Invalid Test
Check Ambient Conditions

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = AMBIENT FAIL
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

AMBIENT FAIL

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 15:58

Test	AC	Time
01 Room Air	0.000	15:58
02 Invalid Sample	X.XXX	15:59
03 Room Air	0.000	15:59

*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INVALID SAMPLE
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

INVALID
SAMPLE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 16:00

Test	AC	Time
01 Room Air	0.000	16:00
02 *Subject Test	ABT*	16:01
03 Room Air	0.000	16:01

*Sequence Aborted

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = SEQ ABORT
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

SEQUENCE
ABORTED

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 16:06

Test	AC	Time
01 Room Air	0.000	16:06
02 Subject Test 1	0.000	16:07
03 Room Air	0.000	16:07
04 Reported AC	0.000	16:07

No RFI Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = ABA TEST
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

ABA TEST

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 16:08

Test	AC	Time
01 Diagnostic	OK	16:09
02 Room Air	0.000	16:10
03 Subject Test 1	0.000	16:10
04 Room Air	0.000	16:12
05 Std. Gas	0.089*	16:13
06 Room Air	0.000	16:14

*Cal Check Out of Tolerance

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = CAL CHK OUT TOL
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
 OUT OF TOLERANCE

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 16:15

Test	AC	Time
01 Diagnostic	OK	16:16
02 Room Air	0.000	16:17
03 *Subject Test	RFI*	16:17
04 Room Air	0.000	16:17

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI DETECTED
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI DETECTED

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 16:18

Test	AC	Time
01 Diagnostic	OK	16:19
02 Room Air	0.000	16:19
03 *Subject Test	0.000*	16:23
04 Room Air	0.000	16:25
05 Std. Gas	0.080	16:26
06 Room Air	0.000	16:27
07 *Subject Test	0.000*	16:30
08 Room Air	0.000	16:31

No RFI Detected

*Deficient Sample - Value Printed was
Highest Obtained

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = DEFICIENT SAMP
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

DEFICIENT
SAMPLES

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 16:31

Test	AC	Time
01 Diagnostic	OK	16:32
02 Room Air	IPS*	16:32
03 Room Air	0.000	16:33

*Improper Sample

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = IMPROPER SAMPLE
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

*IMPROPER
SAMPLE*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 16:34

Test	AC	Time
01 Diagnostic	OK	16:35
02 Room Air	0.000	16:35
03 Subject Test 1	0.100*	16:35
04 Room Air	0.000	16:38
05 Std. Gas	0.081	16:39
06 Room Air	0.000	16:40
07 Subject Test 2	0.247*	16:41
08 Room Air	0.000	16:42

*Difference Too Great

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = DIFF TOO GREAT
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

DIFFERENCE
TOO GREAT

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 16:42

Test	AC	Time
01 Diagnostic	OK	16:43
02 Room Air	0.000	16:44
03 Subject Test 1	0.098	16:44
04 Room Air	0.000	16:46
05 Std. Gas	0.080	16:48
06 Room Air	0.000	16:49
07 Subject Test 2	0.098	16:49
08 Room Air	0.000	16:50
09 Reported AC	0.098	16:49

Difference OK
No RFI Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = CMS TEST
Dr. Lic. = ND/DIS821456
Lot No = 19817080A4
Cyl No = 21
Expiration Date = 09/05/2019
County = 08 Oper No. = 666666

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: CMS MODE

TEST

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007092
Location = TOXL 8164.16.00 09/18
10/11/2018 16:51

Test	AC	Time
01 Room Air	0.000	16:51
02 Std. Gas	0.080	16:52
03 Room Air	0.000	16:52
04 Std. Gas	0.080	16:53
05 Room Air	0.000	16:53
06 Std. Gas	0.081	16:53
07 Room Air	0.000	16:54
08 Std. Gas	0.080	16:54
09 Room Air	0.000	16:55
10 Std. Gas	0.080	16:55
11 Room Air	0.000	16:56
12 Std. Gas	0.080	16:56
13 Room Air	0.000	16:57
14 Std. Gas	0.080	16:57
15 Room Air	0.000	16:57
16 Std. Gas	0.080	16:58
17 Room Air	0.000	16:58
18 Std. Gas	0.081	16:59
19 Room Air	0.000	16:59
20 Std. Gas	0.080	17:00
21 Room Air	0.000	17:00
22 Std. Gas	0.081	17:00
23 Room Air	0.000	17:01
24 Std. Gas	0.080	17:01
25 Room Air	0.000	17:02
26 Std. Gas	0.081	17:02
27 Room Air	0.000	17:03
28 Std. Gas	0.080	17:03
29 Room Air	0.000	17:04
30 Std. Gas	0.081	17:04
31 Room Air	0.000	17:04
32 Std. Gas	0.080	17:05
33 Room Air	0.000	17:05
34 Std. Gas	0.081	17:06
35 Room Air	0.000	17:06
36 Std. Gas	0.081	17:06
37 Room Air	0.000	17:07
38 Std. Gas	0.080	17:07
39 Room Air	0.000	17:08
40 Std. Gas	0.081	17:08
41 Room Air	0.000	17:09
42 Cal Check Stats:		
43 Average	0.0804	
44 Std Dev	0.0005	
45 Rel Std Dev	0.63%	



Operator Signature
CHARLES EDER

Remarks: STABILITY TEST

Form 106-I8000

0.080 AC

LOT: 19817080 A4

CYL: 021

EXP: 9.5.2019