

### INTOXILYZER® 8000 INITIAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-007098

**A. GENERAL Setup and Checks:**

1.  Power On
  - 5 min. countdown during initial warm-up
  - 1 min. countdown to begin test after standby mode
2.  Display Intensity (Ctrl + ↑ or ↓)
3. Password Security:
  - Level 1 (Operator)    Level 2 (Field Inspector)    Level 3 (Lab Personnel)
4.  Printer Setup (Level 3,S,P)
5.  Forms Load (CMI, Inc., CoBrA Software)

**B. LEVEL 1 Setup and Checks:**

1.  Internal Printer Test and Paper Feed (Level 1,P). Attach record.
2.  External Printer Test (Level 1,P). Attach record.
3. Barcode Reader (Level 1,B):
  - Operator ID    ND License    R key: Refusal. Attach record.

**C. LEVEL 2 Setup and Checks:**

1.  Continuous Air Blank (Level 2,A)
2.  Diagnostic (Level 2,D). Attach record.
3.  Prelim Data Entry (Level 2,E)
4. Ser Number/Version Info (Level 2,V):
  - Inst Ser#: 80-007098   DSP Ver: 1362.14
  - Core Ver: 8164.16   CPLD Ver: 7

**D. LEVEL 3 Setup and Checks:**

1. DVM Monitor (Level 3,D,D): 3: 12638 s: 1 C: 47.00  
9: 13278 s: 2 B: 45 0  
(RFI indicator with keyed radio): 1
2. Function (F) Keys: :  F5 – Tone                       F9 - Fan  
 F6 – Green LED                       F10 – Pump  
 F7 – Red LED                           F11 – Solenoid
3. Atmospheric Monitor (Level 3,D,A): Atmo Sensor, P: 963 CF: 1.05
4. Flow Monitor (Level 3,D,F): Flow Sensor, R: 168 F: 0.000 L/s

5. Temperature Monitor (Level 3,D,T): C: 47.0 A: 47.0 I: 0.0  
B: 45.0 V: 0.0
6. Tank Monitor (Level 3,D,G): P (display): 632 psi P (gauge): 600 psi
7.  General Setup (Level 3,S,G)
8.  Configure Start Test (Level 3,S,T)
9.  Network (Level 3,S,N)

**E. TESTS (attach all test records):**

**Configure wet bath simulator standards before running tests (Level 1,S):**

1. Zero AC (Level 1,C):  
Sim ser #: DR3377 Lot #: MILLI Q H<sub>2</sub>O Exp date: NA  
Known value: 0.000 AC  
Results: 0.000 AC 0.000 AC 0.000 AC
2. Low AC (Level 1,C):  
Sim ser #: DR7111 Lot #: 17160 Exp date: 6.8.19  
Known value: 0.020 AC  
Results: 0.019 AC 0.020 AC 0.019 AC
3. High AC (Level 1,C):  
Sim ser #: DR3375 Lot #: 17350 Exp date: 10.11.19  
Known value: 0.300 AC  
Results: 0.296 AC 0.297 AC 0.297 AC

**Configure dry gas standard before running tests (Level 1,S):**

4. Ethanol + 0.05% Acetone (Level 1,B):  
Sim ser #: DR7089 Lot #: ICS 5 Exp date: 5.15.19  
Known value: 0.10 AC + 0.05% ACETONE  
 Display reads "Interferent Detect"
5. Acetone (Level 1,B):  
Sim ser #: DR3846 Lot #: ACE1 Exp date: NA  
Known value: 0.05% ACETONE  
 Display reads "Interferent Detect"
6. Methanol (Level 1,B):  
Sim ser #: DR3455 Lot #: MET2 Exp date: NA  
Known value: 0.10% METHANOL  
 Display reads "Interferent Detect"
7. Isopropanol (Level 1,B):  
Sim ser #: DR5189 Lot #: IPA2 Exp date: NA  
Known value: 0.10% ISOPROPANOL  
 Display reads "Interferent Detect"

- 8.  Ambient Fail (Level 1,B): Display and test record read correct.
- 9.  Invalid Sample (Level 1,B): Display and test record read correct.
- 10.  Sequence Aborted (Level 1,B): Display and test record read correct.
- 11.  ABA (Level 1,B): Test record reads correct.
- 12.  Calibration Check Out of Tolerance (CMS mode): Display and test record read correct.
- 13.  RFI Detected (B,C, or CMS mode): Display and test record read correct.
- 14.  Tank Pressure Below Minimum (CMS mode): Display reads correct.
- 15.  Deficient Samples (CMS mode): Display and test record read correct.
- 16.  Improper Sample (CMS mode): Display and test record read correct.
- 17.  Difference Too Great (CMS mode): Display and test record read correct.
- 18.  CMS (CMS mode): Test record reads correct.
- 19. Stability Test (Level 3,T,S):

Ave: 0.0795 Std Dev: 0.0007 Rel Std Dev: 0.87%

Maintenance/Repairs/Notes: INITIAL INSPECTION AFTER  
RECEIVING INSTRUMENT FROM CMI, INC.

---

---

---

---

---

---

Instrument is acceptable to be used in the field.

Charles E. Edr  
Field Inspector's Signature

10/23/2018  
Date

Roberta Hugo-Norris  
Reviewed by

30 Oct 18  
Date

Intoxilyzer Test Record and Checklist  
NDORAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer  
North Dakota Model 8000 SN 80-007098  
Location = TOXL 8164.16.00 09/18  
10/22/2018 16:42

\*\*\*\*\* Printer Test \*\*\*\*\*

12 char/line  
abcdefghijkl  
ABCDEFGHIJKL

16 char per line  
abcdefghijklmnop  
ABCDEFGHIJKLMNPO

21 chars per line  
abcdefghijklmnopqrstu  
ABCDEFGHIJKLMNOPQRSTU

24 characters per line  
abcdefghijklmnopqrstuvwx  
ABCDEFGHIJKLMNOPQRSTUVWX

32 characters per line  
abcdefghijklmnopqrstuvwxy123456  
ABCDEFGHIJKLMNOPQRSTUVWXY123456

42 characters per line  
abcdefghijklmnopqrstuvwxy1234567890abcdef  
ABCDEFGHIJKLMNOPQRSTUVWXY1234567890ABCDEF

Current Instrument Setup  
Data Entry Mode: Enabled  
Start Test Sequence: DABACABA  
Display Prelim Rslt? Yes  
Display Third Digit? Yes  
Inhib Printer(Y/N)? No  
Display Volume? No  
Disable On Menfull? No  
# of Print Copies? 1  
Select Std (D/W/I)? Dry  
Standard Value? 0.080  
Standard Lot #? 80  
Standard Cyl #? 3456  
Standard Expiration? 11/11/2019  
Oper No? 666666

Flow Cal. Date: 09/26/2018  
Slope 684  
Intercept -588446

IR Calibration Date: 09/26/2018  
3um 9um  
-----  
0th Coef(\*100): -40948 -15551  
1st Coef(\*100): 237555 134140  
2nd Coef(\*100): 2571 1433  
H2O adj(mg/l\*10k): 1097 457

\*\*\*\*\* Test End \*\*\*\*\*



Operator Signature  
CHARLES EDER

Remarks: *Internal  
Print Test*

Form 106-18000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                 8164.16.00 09/18  
10/22/2018                        16:44

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-|=|  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-|=|  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&\*()\_+?

Current Instrument Setup

Data Entry Mode:                Enabled  
Start Test Sequence:            DABACABA  
Display Prelim Rslt?            Yes  
Display Third Digit?            Yes  
Inhib Printer(Y/N)?            No  
Display Volume?                No  
Disable On Memfull?            No  
# of Print Copies?              1  
Select Std (D/W/I)?            Dry  
Standard Value?                0.080  
Standard Lot #?                 80  
Standard Cyl #?                3456  
Standard Expiration?            11/11/2019  
Oper No?                        666666

Flow Cal. Date:                 09/26/2018  
Slope                            684  
Intercept                       -588446

IR Calibration Date:            09/26/2018  
                                    3um                            9um

-----  
0th Coef(\*100):                -40948                        -15551  
1st Coef(\*100):                237555                        134140  
2nd Coef(\*100):                2571                           1433  
H2O adj(mg/l\*10k):            1097                           457

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
CHARLES EDER

Remarks:

EXTERNAL PRINT  
TEST

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007098  
Location = TOXL      8164.16.00 09/18  
10/22/2018      16:45

Test	AC	Time
01 Room Air	0.000	16:46
02 *Subject Test	REF*	16:46
03 Room Air	0.000	16:47

\*Subject Test Refused

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = R KEY REFUSAL  
Dr. Lic. = ND/DIS821456  
Lot No = 80  
Cyl No = 3456  
Expiration Date = 11/11/2019  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: R KEY REFUSAL  
BARCODE READER


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                    8164.16.00 09/18  
10/22/2018                            16:48

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 666666

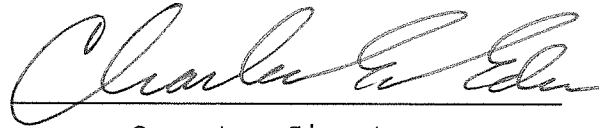

Operator Signature  
CHARLES EDER

Remarks:

DIAGNOSTIC CHECK

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                    8164.16.00 09/18  
10/22/2018                            16:54

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:55
02 Std. Sol.	0.000	16:56
03 Room Air	0.000	16:56
04 Std. Sol.	0.000	16:57
05 Room Air	0.000	16:57
06 Std. Sol.	0.000	16:58
07 Room Air	0.000	16:59

08 Sim Temp = 34.0°C

Simul Ser No = DR3377  
Std Sol No = MILLIQ H2O  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:      ZERO AC  
                    0.000 AC



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                    8164.16.00 09/18  
10/23/2018                            08:51

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:52
02 Std. Sol.	0.019	08:52
03 Room Air	0.000	08:53
04 Std. Sol.	0.020	08:54
05 Room Air	0.000	08:54
06 Std. Sol.	0.019	08:55
07 Room Air	0.000	08:55

08 Sim Temp = 34.0°C

Simul Ser No = DR7111

Std Sol No = 17160

County = 08

Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *Low AC*  
*0.020 AC*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                    8164.16.00 09/18  
10/23/2018                            10:25

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:25
02 Std. Sol.	0.296	10:26
03 Room Air	0.000	10:26
04 Std. Sol.	0.297	10:27
05 Room Air	0.000	10:28
06 Std. Sol.	0.297	10:28
07 Room Air	0.000	10:29


08 Sim Temp = 34.0°C

Simul Ser No = DR3375

Std Sol No = 17350

County = 08

Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

HIGH AC  
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                    8164.16.00 09/18  
10/23/2018                            10:32

Test	AC	Time
01 Room Air	0.000	10:33
02 *Subject Test	INT*	10:33
03 Room Air	0.000	10:34

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = INTERFERENT  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*Interferent Check*  
*0.10AE + 0.05% ACETONE*

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                 8164.16.00 09/18  
10/23/2018                        10:35

Test	AC	Time
01 Room Air	0.000	10:35
02 *Subject Test	INT*	10:36
03 Room Air	0.000	10:36

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                 Weight = 150  
Test = DUI                         Cit = INTERFERENT  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                        Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*Interferent Check*  
*0.05% ACETONE*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                8164.16.00 09/18  
10/23/2018                        10:37

Test	AC	Time
01 Room Air	0.000	10:37
02 *Subject Test	INT*	10:38
03 Room Air	0.000	10:38

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                Weight = 150  
Test = DUI                        Cit = INTERFERENT  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                        Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *Interferent Check*  
*0.10% METHANOL*


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                 8164.16.00 09/18  
10/23/2018                        10:39

Test	AC	Time
01 Room Air	0.000	10:40
02 *Subject Test	INT*	10:41
03 Room Air	0.000	10:41

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = INTERFERENT  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *Interferent Check*  
*0.10% ISOPROPANOL*


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                 8164.16.00 09/18  
10/23/2018                        10:43

Test	AC	Time
01 Room Air	AMB*	10:44
02 Room Air	0.000	10:45

\*Invalid Test  
Check Ambient Conditions

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = AMBIENT FAIL  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*AMBIENT FAIL*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-007098  
Location = TOXL                    8164.16.00 09/18  
10/23/2018                            10:45

Test	AC	Time
01 Room Air	0.000	10:46
02 Invalid Sample	X.XXX	10:46
03 Room Air	0.000	10:47

\*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = INVALID SAMPLE  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *INVALID SAMPLE*



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                    8164.16.00 09/18  
10/23/2018                            10:47

Test	AC	Time
01 Room Air	0.000	10:48
02 *Subject Test	ABT*	10:48
03 Room Air	0.000	10:49

\*Sequence Aborted

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = SEQUENCE ABORT  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

SEQUENCE ABORTED


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                    8164.16.00 09/18  
10/23/2018                            10:49

Test	AC	Time
01 Room Air	0.000	10:50
02 Subject Test 1	0.094	10:50
03 Room Air	0.000	10:51
04 Reported AC	0.094	10:50

No RFI Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = ABA MODE  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *ABA MODE*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                    8164.16.00 09/18  
10/23/2018                            10:52

Test	AC	Time
01 Diagnostic	OK	10:53
02 Room Air	0.000	10:53
03 Subject Test 1	0.094	10:53
04 Room Air	0.000	10:56
05 Std. Gas	0.088*	10:57
06 Room Air	0.000	10:58

\*Cal Check Out of Tolerance

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = CAL CHK OUT TOL  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                            Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
OUT OF TOLERANCE

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                 8164.16.00 09/18  
10/23/2018                        10:59

Test	AC	Time
01 Diagnostic	OK	10:59
02 Room Air	0.000	11:00
03 *Subject Test	RFI*	11:00
04 Room Air	0.000	11:00

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = RFI DETECTED  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                            Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks: *RFI DETECTED*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-007098  
Location = TOXL                    8164.16.00 09/18  
10/23/2018                            11:01

Test	AC	Time
01 Diagnostic	OK	11:02
02 Room Air	0.000	11:03
03 *Subject Test	0.000*	11:06
04 Room Air	0.000	11:08
05 Std. Gas	0.080	11:09
06 Room Air	0.000	11:10
07 *Subject Test	0.000*	11:14
08 Room Air	0.000	11:14
No RFI Detected		

\*Deficient Sample - Value Printed was  
Highest Obtained

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = DEFICIENT SAMP  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                            Oper No. = 666666

20 minute waiting period ascertained? Y  
Clean Mouthpiece used and disposed? Y  
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the  
instructions displayed by the Intoxilyzer  
in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

*DEFICIENT SAMPLES*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                 8164.16.00 09/18  
10/23/2018                        11:28

Test	AC	Time
01 Diagnostic	OK	11:28
02 Room Air	0.000	11:29
03 Reference	IPS*	11:29
04 Room Air	0.000	11:29

\*Improper Sample

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                 Weight = 150  
Test = DUI                         Cit = IMPROPER SAMPLE  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                         Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks: *IMPROPER SAMPLE*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                 8164.16.00 09/18  
10/23/2018                        11:30

Test	AC	Time
01 Diagnostic	OK	11:31
02 Room Air	0.000	11:31
03 Subject Test 1	0.243*	11:32
04 Room Air	0.000	11:34
05 Std. Gas	0.079	11:35
06 Room Air	0.000	11:37
07 Subject Test 2	0.095*	11:37
08 Room Air	0.000	11:38

\*Difference Too Great

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = DIFF TOO GREAT  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                            Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

DIFFERENCE  
TOO GREAT

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007098  
Location = TOXL                 8164.16.00 09/18  
10/23/2018                        11:39


Test	AC	Time
01 Diagnostic	OK	11:40
02 Room Air	0.000	11:40
03 Subject Test 1	0.096	11:41
04 Room Air	0.000	11:43
05 Std. Gas	0.079	11:44
06 Room Air	0.000	11:45
07 Subject Test 2	0.093	11:46
08 Room Air	0.000	11:46
09 Reported AC	0.093	11:46

Difference OK  
No RFI Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = CMS MODE  
Dr. Lic. = ND/DIS821456  
Lot No = 17618080A1  
Cyl No = 28  
Expiration Date = 08/05/2020  
County = 08                            Oper No. = 666666

20 minute waiting period ascertained? Y  
Clean Mouthpiece used and disposed? Y  
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the  
instructions displayed by the Intoxilyzer  
in conducting this test.

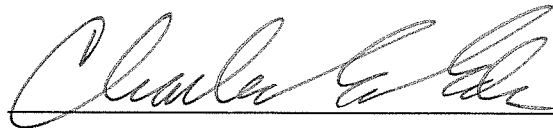

Operator Signature  
CHARLES EDER

Remarks: *CMS MODE*



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007098  
Location = TOXL      8164.16.00 09/18  
10/23/2018      11:47

Test	AC	Time
01 Room Air	0.000	11:48
02 Std. Gas	0.079	11:48
03 Room Air	0.000	11:48
04 Std. Gas	0.080	11:49
05 Room Air	0.000	11:49
06 Std. Gas	0.079	11:50
07 Room Air	0.000	11:50
08 Std. Gas	0.080	11:51
09 Room Air	0.000	11:51
10 Std. Gas	0.080	11:51
11 Room Air	0.000	11:52
12 Std. Gas	0.079	11:52
13 Room Air	0.000	11:53
14 Std. Gas	0.080	11:53
15 Room Air	0.000	11:54
16 Std. Gas	0.078	11:54
17 Room Air	0.000	11:54
18 Std. Gas	0.079	11:55
19 Room Air	0.000	11:55
20 Std. Gas	0.079	11:56
21 Room Air	0.000	11:56
22 Std. Gas	0.079	11:57
23 Room Air	0.000	11:57
24 Std. Gas	0.080	11:57
25 Room Air	0.000	11:58
26 Std. Gas	0.080	11:58
27 Room Air	0.000	11:59
28 Std. Gas	0.081	11:59
29 Room Air	0.000	12:00
30 Std. Gas	0.080	12:00
31 Room Air	0.000	12:01
32 Std. Gas	0.079	12:01
33 Room Air	0.000	12:01
34 Std. Gas	0.079	12:02
35 Room Air	0.000	12:02
36 Std. Gas	0.080	12:03
37 Room Air	0.000	12:03
38 Std. Gas	0.080	12:04
39 Room Air	0.000	12:04
40 Std. Gas	0.079	12:04
41 Room Air	0.000	12:05
42 Cal Check Stats:		
43 Average	0.0795	
44 Std Dev	0.0007	
45 Rel Std Dev	0.87%	



Operator Signature  
CHARLES EDER

Remarks: STABILITY  
TEST

Form 106-I8000

0.080 AC

LOT: 17618080A1

CYL: 028

EXP: 8/5/2020