





Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007095  
Location = HETT      8164.16.00 09/18  
04/12/2019      12:13

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:14
02 Std. Sol.	0.018	12:15
03 Room Air	0.000	12:15
04 Std. Sol.	0.018	12:16
05 Room Air	0.000	12:17
06 Std. Sol.	0.018	12:17
07 Room Air	0.000	12:18
08 Sim Temp = 34.0°C		

Simul Ser No = DR3375

Std Sol No = 17160

County = 01

Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

Low AC  
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007095  
Location = HETT      8164.16.00 09/18  
04/12/2019      12:31

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:32
02 Std. Sol.	0.300	12:32
03 Room Air	0.000	12:33
04 Std. Sol.	0.301	12:34
05 Room Air	0.000	12:34
06 Std. Sol.	0.301	12:35
07 Room Air	0.000	12:35

08 Sim Temp = 34.0°C

Simul Ser No = DR7111

Std Sol No = 17350

County = 01

Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

HIGH AC  
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007095  
Location = HETT      8164.16.00 09/18  
04/12/2019      12:03

Test	AC	Time
01 Room Air	0.000	12:04
02 *Subject Test	INT*	12:04
03 Room Air	0.000	12:05

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = INTERFERENT  
Dr. Lic. = ND/DIS821456  
Lot No = 34917080A3  
Cyl No = 14  
Expiration Date = 02/05/2020  
County = 01      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*Interferent Check*  
*0.10AC + 0.05% ACETONE*  
Form 106-I8000.

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007095  
Location = HETT      8164.16.00 09/18  
04/12/2019      12:06

Test	AC	Time
01 Diagnostic	OK	12:07
02 Room Air	0.000	12:07
03 *Subject Test	RFI*	12:08
04 Room Air	0.000	12:08

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = RFI CHECK  
Dr. Lic. = ND/DIS821456  
Lot No = 34917080A3  
Cyl No = 14  
Expiration Date = 02/05/2020  
County = 01      Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

*RFI CHECK*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007095  
Location = HETT      8164.16.00 09/18  
04/12/2019      11:59

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:59
02 Std. Gas	0.082	12:00
03 Room Air	0.000	12:00
04 Std. Gas	0.082	12:01
05 Room Air	0.000	12:01
06 Std. Gas	0.081	12:01
07 Room Air	0.000	12:02

Lot No = 34917080A3  
Cyl No = 14  
Exp Date = 02/05/2020  
County = 01

Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

CALIBRATION CHECK  
0.080AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007095  
Location = HETT      8164.16.00 09/18  
04/12/2019      12:37

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:38
02 Std. Gas	0.082	12:38
03 Room Air	0.000	12:39
04 Std. Gas	0.082	12:39
05 Room Air	0.000	12:39
06 Std. Gas	0.082	12:40
07 Room Air	0.000	12:40

Lot No = 34917080A3  
Cyl No = 14  
Exp Date = 02/05/2020  
County = 01

Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*CALIBRATION CHECK*  
*0.104 CEE 0.080 AC*

Form 106-I8000



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007095  
Location = HETT      8164.16.00 09/18  
04/12/2019      12:40

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:41
02 Std. Gas	0.081	12:41
03 Room Air	0.000	12:42
04 Std. Gas	0.081	12:42
05 Room Air	0.000	12:43
06 Std. Gas	0.082	12:43
07 Room Air	0.000	12:44

Lot No = 34917080A3  
Cyl No = 14  
Exp Date = 02/05/2020  
County = 01

Oper No. = 666666

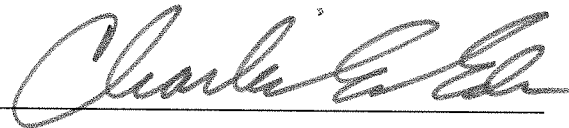

Operator Signature  
CHARLES EDER

Remarks:

*CALIBRATION CHECK*  
*0.080 AC*

Form 106-I8000