

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-007096

Location: TOXL

A. General Setup and Checks:

1.  Diagnostic Tests Pass and Instrument in Ready Mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
  - a. Display: 247 psi Regulator: 250 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a.  Low AC (Level 1,C): Known Value  $\leq 0.03$  AC: 0.020 AC  
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2-13-22
- b.  High AC (Level 1,C): Known Value  $\geq 0.25$  AC: 0.300 AC  
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12-8-22

Configure dry gas standard for the following tests (Level 1,S).

2.  Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR3847 Lot #: ICS 6 Exp. Date: NA  
 Display reads "Interferent Detect"
3.  RFI Check (CMS Mode)  Display reads "RFI Detect"
4.  Dry Calibration Check (Level 1,C): Known Value 0.080 AC  
Gas Cyl Lot #: 02621080A1 Cyl #: 25 Exp. Date: 3-5-23

Test 1	<u>0.080</u>	Test 4	<u>0.080</u>	Test 7	<u>0.080</u>
Test 2	<u>0.080</u>	Test 5	<u>0.080</u>	Test 8	<u>0.080</u>
Test 3	<u>0.080</u>	Test 6	<u>0.081</u>	Test 9	<u>0.080</u>
Average	<u>0.080</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Breath Analyst Signature

Reviewed by

Date

Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-007096  
Location = TOXL                 8164.16.00 09/18  
04/21/2021                        14:55

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^\*()\_+?

Current Instrument Setup


Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?         1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            02621080A1  
Standard Cyl #?            25  
Standard Expiration?       03/05/2023  
Oper No?                    666666

Flow Cal. Date:            10/02/2018  
Slope                        695  
Intercept                   -692605

IR Calibration Date:        10/02/2018

	3um	9um
0th Coef(*100):	-33544	-18475
1st Coef(*100):	261464	138054
2nd Coef(*100):	3020	1612
H2O adj(mg/l*10k):	573	386

\*\*\*\*\* Printer Test End \*\*\*\*\*

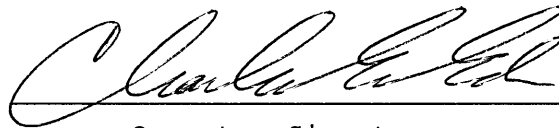

Operator Signature  
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007096  
Location = TOXL      8164.16.00 09/18  
04/21/2021      14:58

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:58
02 Std. Sol.	0.018	14:59
03 Room Air	0.000	15:00
04 Std. Sol.	0.018	15:00
05 Room Air	0.000	15:01
06 Std. Sol.	0.018	15:02
07 Room Air	0.000	15:02

08 Sim Temp = 34.0°C

Simul Ser No = MP3064  
Std Sol No = 20070  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *Low AC*  
*0.020 AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007096  
Location = TOXL      8164.16.00 09/18  
04/21/2021      15:04

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:05
02 Std. Sol.	0.301	15:05
03 Room Air	0.000	15:06
04 Std. Sol.	0.302	15:07
05 Room Air	0.000	15:07
06 Std. Sol.	0.302	15:08
07 Room Air	0.000	15:09

08 Sim Temp = 34.0°C

Simul Ser No = MP5317  
Std Sol No = 2020121A  
County = 08      Oper No. = 666666

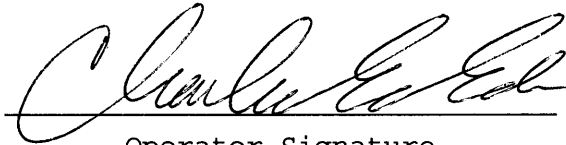

Operator Signature  
CHARLES EDER

Remarks: HIGH AC  
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007096  
Location = TOXL      8164.16.00 09/18  
04/21/2021      15:11

Test	AC	Time
01 Room Air	0.000	15:12
02 *Subject Test	INT*	15:12
03 Room Air	0.000	15:13

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 02/01/1992  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = INTERFERENT  
Dr. Lic. = ND/DIS921456  
Lot No = 02621080A1  
Cyl No = 25  
Expiration Date = 03/05/2023  
County = 08      Oper No. = 666666

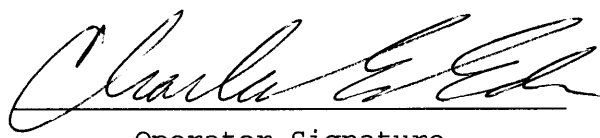

Operator Signature  
CHARLES EDER

Remarks: *Interferent Check*  
*0.10 AC + 0.05% ACETONE*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007096  
Location = TOXL      8164.16.00 09/18  
04/21/2021      15:14

Test	AC	Time
01 Diagnostic	OK	15:15
02 Room Air	0.000	15:15
03 *Subject Test	RFI*	15:15
04 Room Air	0.000	15:16

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 02/01/1992  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = RFI CHECK  
Dr. Lic. = ND/DIS921456  
Lot No = 02621080A1  
Cyl No = 25  
Expiration Date = 03/05/2023  
County = 08      Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks: *RFI CHECK*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007096  
Location = TOXL      8164.16.00 09/18  
04/21/2021      15:16

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:16
02 Std. Gas	0.080	15:17
03 Room Air	0.000	15:17
04 Std. Gas	0.080	15:18
05 Room Air	0.000	15:18
06 Std. Gas	0.080	15:18
07 Room Air	0.000	15:19

Lot No = 02621080A1  
Cyl No = 25  
Exp Date = 03/05/2023  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007096  
Location = TOXL      8164.16.00 09/18  
04/21/2021      15:20

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:20
02 Std. Gas	0.080	15:21
03 Room Air	0.000	15:21
04 Std. Gas	0.080	15:22
05 Room Air	0.000	15:22
06 Std. Gas	0.081	15:22
07 Room Air	0.000	15:23

Lot No = 02621080A1  
Cyl No = 25  
Exp Date = 03/05/2023  
County = 08      Oper No. = 666666

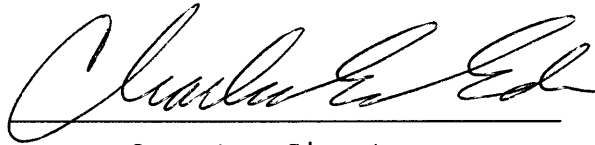

Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007096  
Location = TOXL      8164.16.00 09/18  
04/21/2021      15:23

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:24
02 Std. Gas	0.080	15:24
03 Room Air	0.000	15:25
04 Std. Gas	0.080	15:25
05 Room Air	0.000	15:26
06 Std. Gas	0.080	15:26
07 Room Air	0.000	15:26

Lot No = 02621080A1  
Cyl No = 25  
Exp Date = 03/05/2023  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000