

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-007091

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 877 psi Regulator: 900 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.015 AC
Sim. Ser #: MP5319 Lot #: 201911C Exp. Date: 11-19-21
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.400 AC
Sim. Ser #: MP3060 Lot #: 1910B Exp. Date: 10-20-21

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR7348 Lot #: 1C95 Exp. Date: NA

Display reads "Interferent Detect"

3. RFI Check (CMS Mode) Display reads "RFI Detect"

4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC

Gas Cyl Lot #: 02621080A Cyl #: WH026041 Exp. Date: 3-5-23 4-05-2022 WH

Test 1	<u>0.080</u>	Test 4	<u>0.0801</u>	Test 7	<u>0.081</u>
Test 2	<u>0.080</u>	Test 5	<u>0.080</u>	Test 8	<u>0.081</u>
Test 3	<u>0.080</u>	Test 6	<u>0.080</u>	Test 9	<u>0.080</u>
Average	<u>0.080</u>				

C. Remarks/Maintenance: Annual Inspection

kept time as Mountain Time. Replaced gas regulator.

Instrument is acceptable to be used in the field.

Kari L. Hiet
Breath Analyst Signature

5-3-21
Date

Charles E. Ed
Reviewed by

5.3.21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
05/03/2021 13:01

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 05620080A1
Standard Cyl #? 41
Standard Expiration? 04/05/2022
Oper No? 132598

Flow Cal. Date: 09/25/2018
Slope 681
Intercept -651030

IR Calibration Date: 09/25/2018
 3um 9um

0th Coef(*100):	-39121	-20906
1st Coef(*100):	240667	132345
2nd Coef(*100):	3960	1516
H2O adj(mg/l*10k):	899	428

***** Printer Test End *****

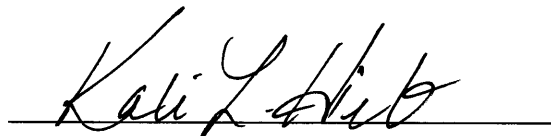

Operator Signature
KALI HIEB

Remarks: *print test*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
05/03/2021 13:13

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:13
02 Std. Sol.	0.013	13:14
03 Room Air	0.000	13:15
04 Std. Sol.	0.013	13:15
05 Room Air	0.000	13:16
06 Std. Sol.	0.014	13:17
07 Room Air	0.000	13:17

08 Sim Temp = 34.0°C

Simul Ser No = MP5319
Std Sol No = 201911C
County = 08 Oper No. = 132598

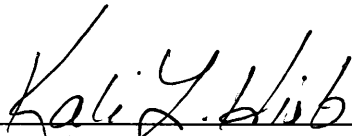

Operator Signature
KALI HIEB

Remarks: *low cal check 0.015AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
05/03/2021 13:19

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:20
02 Std. Sol.	0.405	13:21
03 Room Air	0.000	13:21
04 Std. Sol.	0.408	13:22
05 Room Air	0.000	13:22
06 Std. Sol.	0.408	13:23
07 Room Air	0.000	13:24

08 Sim Temp = 33.9°C

Simul Ser No = MP3060
Std Sol No = 19108
County = 08 Oper No. = 132598

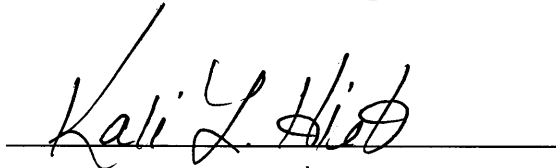
Operator Signature
KALI HIEB

Remarks: *High ac cal check 0.400 ac*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
05/03/2021 13:26

Test	AC	Time
01 Room Air	0.000	13:27
02 *Subject Test	INT*	13:27
03 Room Air	0.000	13:28

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 026
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

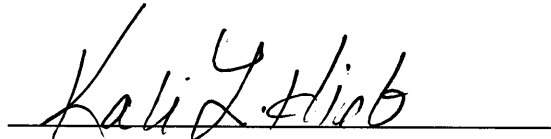

Operator Signature
KALI HIEB

Remarks: *Interferent Check*
0.10AC & 0.05% Acetone
Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
05/03/2021 13:29

Test	AC	Time
01 Diagnostic	OK	13:29
02 Room Air	0.000	13:30
03 Reference	RFI*	13:30
04 Room Air	0.000	13:30

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 026
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

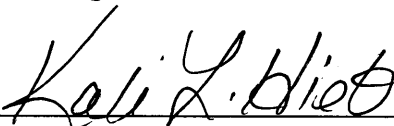

Operator Signature
KALI HIEB

Remarks: *RFI check*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
05/03/2021 14:05

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:05
02 Std. Gas	0.080	14:06
03 Room Air	0.000	14:06
04 Std. Gas	0.080	14:07
05 Room Air	0.000	14:07
06 Std. Gas	0.080	14:08
07 Room Air	0.000	14:08

Lot No = 05620080A1
Cyl No = 41
Exp Date = 04/05/2022
County = 08 Oper No. = 132598

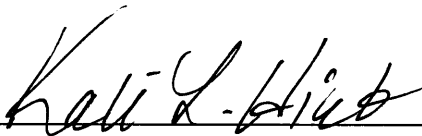

Operator Signature
KALI HIEB

Remarks: *cal check 0.080 AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
05/03/2021 14:09

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:10
02 Std. Gas	0.081	14:10
03 Room Air	0.000	14:10
04 Std. Gas	0.080	14:11
05 Room Air	0.000	14:11
06 Std. Gas	0.080	14:12
07 Room Air	0.000	14:12

Lot No = 05620080A1
Cyl No = 41
Exp Date = 04/05/2022
County = 08 Oper No. = 132598

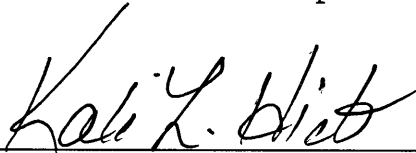

Operator Signature
KALI HIEB

Remarks: *cal check 0.080AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
05/03/2021 14:13

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:14
02 Std. Gas	0.081	14:14
03 Room Air	0.000	14:15
04 Std. Gas	0.081	14:15
05 Room Air	0.000	14:16
06 Std. Gas	0.080	14:16
07 Room Air	0.000	14:16

Lot No = 05620080A1
Cyl No = 41
Exp Date = 04/05/2022
County = 08 Oper No. = 132598


Operator Signature
KALI HIEB

Remarks: *cal check 0.000 AC*

Form 106-I8000