

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-007095

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 227 psi Regulator: 225 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICS6 Exp. Date: NA

Display reads "Interferent Detect"

3. RFI Check (CMS Mode) Display reads "RFI Detect"

4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC

Gas Cyl Lot #: 02621080A Cyl #: 25 Exp. Date: 3.5.23

Test 1 0.083 Test 4 0.082 Test 7 0.083

Test 2 0.083 Test 5 0.082 Test 8 0.082

Test 3 0.083 Test 6 0.082 Test 9 0.082

Average 0.082

C. Remarks/Maintenance: ANNUAL INSPECTION, REPLACED
EXTERNAL BATTERY.

LEFT ON MOUNTAIN TIME FOR INSPECTION.

Instrument is acceptable to be used in the field.

Charles E. Eder
Breath Analyst Signature

5.6.2021
Date

Kali J. Hoot
Reviewed by

5-11-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007095
Location = TOXL 8164.16.00 09/18
05/06/2021 08:34

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNQPQRSTUVWXYZ!@#%&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNQPQRSTUVWXYZ!@#%&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 25
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 09/27/2018
Slope 683
Intercept -637452

IR Calibration Date: 09/27/2018

	3um	9um
0th Coef(*100):	-59629	-23097
1st Coef(*100):	252379	137307
2nd Coef(*100):	2489	1549
H2O adj(mg/l*10k):	1414	594

***** Printer Test End *****

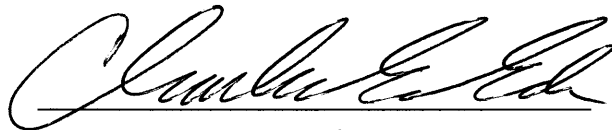

Operator Signature

CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007095
Location = TOXL 8164.16.00 09/18
05/06/2021 08:34

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:35
02 Std. Sol.	0.017	08:36
03 Room Air	0.000	08:36
04 Std. Sol.	0.018	08:37
05 Room Air	0.000	08:37
06 Std. Sol.	0.018	08:38
07 Room Air	0.000	08:39

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

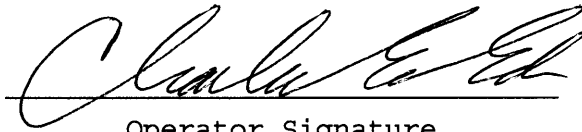

Operator Signature
CHARLES EDER

Remarks:

Low AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007095
Location = TOXL 8164.16.00 09/18
05/06/2021 08:40

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:41
02 Std. Sol.	0.302	08:41
03 Room Air	0.000	08:42
04 Std. Sol.	0.303	08:43
05 Room Air	0.000	08:43
06 Std. Sol.	0.302	08:44
07 Room Air	0.000	08:44

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666

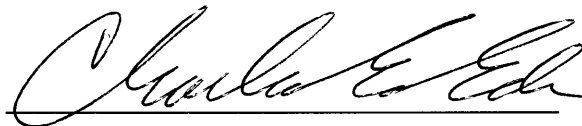

Operator Signature
CHARLES EDER

Remarks: *HIGH AC*
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007095
Location = TOXL 8164.16.00 09/18
05/06/2021 08:47

Test	AC	Time
01 Room Air	0.000	08:47
02 *Subject Test	INT*	08:48
03 Room Air	0.000	08:48

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

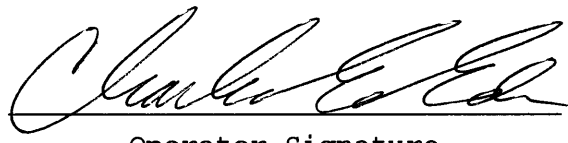

Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10AC + 0.05% ACETONE

Form 106-18000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007095
Location = TOXL 8164.16.00 09/18
05/06/2021 08:49

Test	AC	Time
01 Diagnostic	OK	08:50
02 Room Air	0.000	08:51
03 *Subject Test	RFI*	08:51
04 Room Air	0.000	08:51

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *RFI CHECK*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007095
Location = TOXL 8164.16.00 09/18
05/06/2021 08:52

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:52
02 Std. Gas	0.083	08:53
03 Room Air	0.000	08:53
04 Std. Gas	0.083	08:54
05 Room Air	0.000	08:54
06 Std. Gas	0.083	08:54
07 Room Air	0.000	08:55

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007095
Location = TOXL 8164.16.00 09/18
05/06/2021 08:55

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:56
02 Std. Gas	0.082	08:56
03 Room Air	0.000	08:57
04 Std. Gas	0.082	08:57
05 Room Air	0.000	08:58
06 Std. Gas	0.082	08:58
07 Room Air	0.000	08:58

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

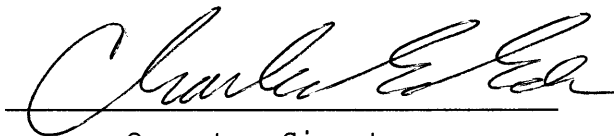

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007095
Location = TOXL 8164.16.00 09/18
05/06/2021 09:10

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:11
02 Std. Gas	0.083	09:11
03 Room Air	0.000	09:12
04 Std. Gas	0.082	09:12
05 Room Air	0.000	09:13
06 Std. Gas	0.082	09:13
07 Room Air	0.000	09:13

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

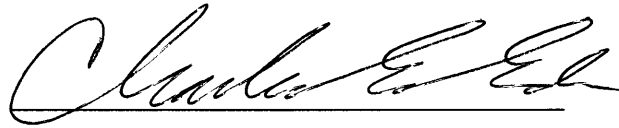

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000