

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-007093

Location: TOL

A. General Setup and Checks:

1.  Diagnostic Tests Pass and Instrument in Ready Mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
  - a. Display: 967 psi Regulator: 950 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a.  Low AC (Level 1,C): Known Value  $\leq 0.03$  AC: 0.030 AC  
Sim. Ser #: MP5289 Lot #: 201911E Exp. Date: 11-19-21
- b.  High AC (Level 1,C): Known Value  $\geq 0.25$  AC: 0.400 AC  
Sim. Ser #: MP3062 Lot #: 202103E Exp. Date: 3-24-23

Configure dry gas standard for the following tests (Level 1,S).

2.  Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone  
Sim. Ser #: DR3847 Lot #: ICS 6 Exp. Date: NA

Display reads "Interferent Detect"

3.  RFI Check (CMS Mode)  Display reads "RFI Detect"
4.  Dry Calibration Check (Level 1,C): Known Value 0.080 AC

Gas Cyl Lot #: 05620080A1 Cyl #: 48 Exp. Date: 4-5-22

Test 1	<u>0.081</u>	Test 4	<u>0.081</u>	Test 7	<u>0.080</u>
Test 2	<u>0.079</u>	Test 5	<u>0.080</u>	Test 8	<u>0.080</u>
Test 3	<u>0.080</u>	Test 6	<u>0.080</u>	Test 9	<u>0.080</u>
Average	<u>0.080</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION,

INSTRUMENT LEFT ON MOUNTAIN TIME FOR INSPECTION.

Instrument is acceptable to be used in the field.

Charles E. Ehr  
Breath Analyst Signature

5/17/21  
Date

Kari L. Hieb  
Reviewed by

5-17-21  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-007093  
Location = TOXL                    8164.16.00 09/18  
05/17/2021                            08:04

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&\*()\_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&\*()\_+?

Current Instrument Setup

Data Entry Mode:                    Enabled  
Start Test Sequence:                DABACABA  
Display Prelim Rslt?                Yes  
Display Third Digit?                Yes  
Inhib Printer(Y/N)?                No  
Display Volume?                    No  
Disable On Memfull?                Yes  
# of Print Copies?                  1  
Select Std (D/W/I)?                Dry  
Standard Value?                    0.080  
Standard Lot #?                    24119080A1  
Standard Cyl #?                    33  
Standard Expiration?                11/05/2021  
Oper No?                            666666

Flow Cal. Date:                    06/07/2019  
Slope                                638  
Intercept                            -611758

IR Calibration Date:                12/16/2019  
    3um                                9um

-----  
0th Coef(\*100):                    -14610                                -32356  
1st Coef(\*100):                    264615                                138933  
2nd Coef(\*100):                    2992                                    1364  
H2O adj(mg/l\*10k):                369                                    621

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
CHARLES EDER

Remarks:                    PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007093  
Location = TOXL      8164.16.00 09/18  
05/17/2021      08:21

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:22
02 Std. Sol.	0.027	08:23
03 Room Air	0.000	08:23
04 Std. Sol.	0.026	08:24
05 Room Air	0.000	08:25
06 Std. Sol.	0.027	08:25
07 Room Air	0.000	08:26


08 Sim Temp = 34.0°C

Simul Ser No = MP5289

Std Sol No = 201911E

County = 08

Oper No. = 666666

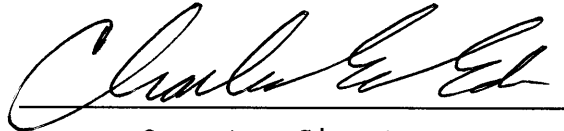

Operator Signature

CHARLES EDER

Remarks:

LOW AC  
0.030 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007093  
Location = TOXL      8164.16.00 09/18  
05/17/2021      08:29

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:30
02 Std. Sol.	0.391	08:31
03 Room Air	0.000	08:31
04 Std. Sol.	0.392	08:32
05 Room Air	0.000	08:33
06 Std. Sol.	0.392	08:33
07 Room Air	0.000	08:34

08 Sim Temp = 34.0°C

Simul Ser No = MP3062  
Std Sol No = 202103E  
County = 08      Oper No. = 666666

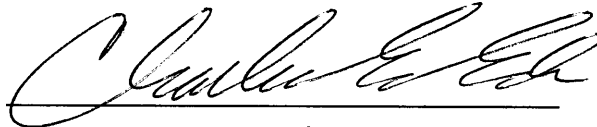

Operator Signature  
CHARLES EDER

Remarks:

HIGH AC  
0.400 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007093  
Location = TOXL      8164.16.00 09/18  
05/17/2021      08:38

Test	AC	Time
01 Room Air	0.000	08:39
02 *Subject Test	INT*	08:39
03 Room Air	0.000	08:40

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/08/1987  
Sub Sex = Male      Weight = 150  
Test = DUI      Cit = INTERFERENT  
Dr. Lic. = ND/DIS871456  
Lot No = 05620080A1  
Cyl No = 48  
Expiration Date = 04/05/2022  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*Interferant Check*  
*0.10AC + 0.05% ACETONE*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-007093  
Location = TOXL                    8164.16.00 09/18  
05/17/2021                            08:40

Test	AC	Time
01 Diagnostic	OK	08:41
02 Room Air	0.000	08:41
03 *Subject Test	RFI*	08:42
04 Room Air	0.000	08:42

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/08/1987  
Sub Sex = Male                            Weight = 150  
Test = DUI                                Cit = RFI CHECK  
Dr. Lic. = ND/DIS871456  
Lot No = 05620080A1  
Cyl No = 48  
Expiration Date = 04/05/2022  
County = 08                                Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

*RFI CHECK*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007093  
Location = TOXL      8164.16.00 09/18  
05/17/2021      08:42

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:43
02 Std. Gas	0.081	08:43
03 Room Air	0.000	08:44
04 Std. Gas	0.079	08:44
05 Room Air	0.000	08:45
06 Std. Gas	0.080	08:45
07 Room Air	0.000	08:46

Lot No = 05620080A1  
Cyl No = 48  
Exp Date = 04/05/2022  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

CALIBRATION CHECK  
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007093  
Location = TOXL      8164.16.00 09/18  
05/17/2021      08:46

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:47
02 Std. Gas	0.081	08:47
03 Room Air	0.000	08:47
04 Std. Gas	0.080	08:48
05 Room Air	0.000	08:48
06 Std. Gas	0.080	08:49
07 Room Air	0.000	08:49

Lot No = 05620080A1  
Cyl No = 48  
Exp Date = 04/05/2022  
County = 08      Oper No. = 666666

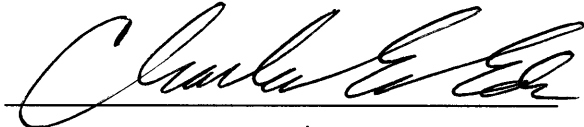

Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-007093  
Location = TOXL      8164.16.00 09/18  
05/17/2021      08:50

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:50
02 Std. Gas	0.080	08:51
03 Room Air	0.000	08:51
04 Std. Gas	0.080	08:51
05 Room Air	0.000	08:52
06 Std. Gas	0.080	08:52
07 Room Air	0.000	08:53

Lot No = 05620080A1  
Cyl No = 48  
Exp Date = 04/05/2022  
County = 08      Oper No. = 666666

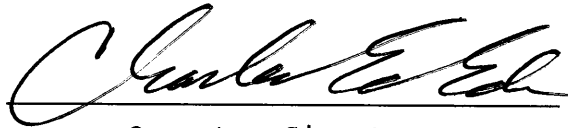

Operator Signature  
CHARLES EDER

Remarks:

*CALIBRATION CHECK*  
*0.080 AC*

Form 106-I8000