

INTOXILYZER® 8000 INITIAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-007091

A. GENERAL Setup and Checks:

1. Power On
 5 min. countdown during initial warm-up
 1 min. countdown to begin test after standby mode
2. Display Intensity (Ctrl + ↑ or ↓)
3. Password Security:
 Level 1 (Operator) Level 2 (Field Inspector) Level 3 (Lab Personnel)
4. Printer Setup (Level 3,S,P)
5. Forms Load (CMI, Inc., CoBrA Software)

B. LEVEL 1 Setup and Checks:

1. Internal Printer Test and Paper Feed (Level 1,P). Attach record.
2. External Printer Test (Level 1,P). Attach record.
3. Barcode Reader (Level 1,B):
 Operator ID ND License R key: Refusal. Attach record.

C. LEVEL 2 Setup and Checks:

1. Continuous Air Blank (Level 2,A)
2. Diagnostic (Level 2,D). Attach record.
3. Prelim Data Entry (Level 2,E)
4. Ser Number/Version Info (Level 2,V):
Inst Ser#: 80-007091 DSP Ver: CEE ~~137~~ 1362.14
Core Ver: 8164.16 CPLD Ver: 7

D. LEVEL 3 Setup and Checks:

1. DVM Monitor (Level 3,D,D): 3: 12488 s: 0 c: 47.00
9: 13910 s: 1 B: 45 0
(RFI indicator with keyed radio): 1
2. Function (F) Keys : F5 – Tone F9 - Fan
 F6 – Green LED F10 – Pump
 F7 – Red LED F11 – Solenoid
3. Atmospheric Monitor (Level 3,D,A): Atmo Sensor, P: 964 CF: 1.05
4. Flow Monitor (Level 3,D,F): Flow Sensor, R: 200 F: 0.000 L/s

5. Temperature Monitor (Level 3,D,T): C: 47.0 A: 47.5 I: 0.0
B: 45.0 V: 0.0
6. Tank Monitor (Level 3,D,G): P (display): 627 psi P (gauge): 650 psi
7. General Setup (Level 3,S,G)
8. Configure Start Test (Level 3,S,T)
9. Network (Level 3,S,N)

E. TESTS (attach all test records):

Configure wet bath simulator standards before running tests (Level 1,S):

1. Zero AC (Level 1,C):
Sim ser #: DR3377 Lot #: MILLI Q H₂O Exp date: NA
Known value: 0.000 AC
Results: 0.000 AC 0.000 AC 0.000 AC
2. Low AC (Level 1,C):
Sim ser #: DR 7111 Lot #: 17160 Exp date: 6.8.19
Known value: 0.020 AC
Results: 0.019 AC 0.019 AC 0.018 AC
3. High AC (Level 1,C):
Sim ser #: DR 3375 Lot #: 17350 Exp date: 10.11.19
Known value: 0.300 AC
Results: 0.296 AC 0.296 AC 0.296 AC

Configure dry gas standard before running tests (Level 1,S):

4. Ethanol + 0.05% Acetone (Level 1,B):
Sim ser #: DR 7089 Lot #: ICS #5 Exp date: 5.15.19
Known value: 0.10 AC + 0.05% ACETONE
 Display reads "Interferent Detect"
5. Acetone (Level 1,B):
Sim ser #: DR 3846 Lot #: ACE 1 Exp date: NA
Known value: 0.05% ACETONE
 Display reads "Interferent Detect"
6. Methanol (Level 1,B):
Sim ser #: DR 3455 Lot #: MET 2 Exp date: NA
Known value: ~~0.05%~~ 0.10% METHANOL
 Display reads "Interferent Detect"
7. Isopropanol (Level 1,B):
Sim ser #: DR 5189 Lot #: IPA 2 Exp date: NA
Known value: 0.10% ISOPROPANOL
 Display reads "Interferent Detect"

- 8. Ambient Fail (Level 1,B): Display and test record read correct.
- 9. Invalid Sample (Level 1,B): Display and test record read correct.
- 10. Sequence Aborted (Level 1,B): Display and test record read correct.
- 11. ABA (Level 1,B): Test record reads correct.
- 12. Calibration Check Out of Tolerance (CMS mode): Display and test record read correct.
- 13. RFI Detected (B,C, or CMS mode): Display and test record read correct.
- 14. Tank Pressure Below Minimum (CMS mode): Display reads correct.
- 15. Deficient Samples (CMS mode): Display and test record read correct.
- 16. Improper Sample (CMS mode): Display and test record read correct.
- 17. Difference Too Great (CMS mode): Display and test record read correct.
- 18. CMS (CMS mode): Test record reads correct.
- 19. Stability Test (Level 3,T,S):


Ave: 0.0798 Std Dev: 0.0006 Rel Std Dev: 0.81%

Maintenance/Repairs/Notes: INITIAL INSPECTION AFTER FIRMWARE
UPDATE ON INTERNAL PRINTER AT CMI, INC. FACTORY.

Instrument is acceptable to be used in the field.


Field Inspector's Signature

11/8/2018
Date


Reviewed by

9 Nov 18
Date

Intoxilyzer Test Record and Checklist
NDORAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 11:21

***** Printer Test *****

12 char/line
abcdefghijkl
ABCDEFGHIJKL

16 char per line
abcdefghijklmnop
ABCDEFGHIJKLMN

21 chars per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNOPQR

24 characters per line
abcdefghijklmnopqrstuvwx
ABCDEFGHIJKLMNOPQR

32 characters per line
abcdefghijklmnopqrstuvwxy123456
ABCDEFGHIJKLMNOPQR

42 characters per line
abcdefghijklmnopqrstuvwxy1234567890abcdef
ABCDEFGHIJKLMNOPQR

Current Instrument Setup
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On MenFull? No
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.081
Standard Lot #? 81
Standard Cyl #? 1111
Standard Expiration? 11/11/2019
Oper No? 666666

Flow Cal. Date: 09/25/2018
Slope 681
Intercept -651030

IR Calibration Date: 09/25/2018
3um 9um

0th Coef(*100): -39121 -20906

1st Coef(*100): 240667 132345

2nd Coef(*100): 3960 1516

H2O adj(mg/l*10k): 899 428

***** Test End *****



Operator Signature
CHARLES EDER

Remarks:

*Internal
PRINT TEST*

Form 106-18000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 11:25

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-|=|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-|=|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? No
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.081
Standard Lot #? 81
Standard Cyl #? 1111
Standard Expiration? 11/11/2019
Oper No? 666666

Flow Cal. Date: 09/25/2018
Slope 681
Intercept -651030

IR Calibration Date: 09/25/2018
 3um 9um

0th Coef(*100): -39121 -20906
1st Coef(*100): 240667 132345
2nd Coef(*100): 3960 1516
H2O adj(mg/l*10k): 899 428

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks: *EXTERNAL*
 PRINT TEST

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 11:26

Test	AC	Time
01 Room Air	0.000	11:27
02 *Subject Test	REF*	11:27
03 Room Air	0.000	11:28

*Subject Test Refused

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = R KEY REFUSAL
Dr. Lic. = ND/DIS821456
Lot No = 81
Cyl No = 1111
Expiration Date = 11/11/2019
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: R KEY REFUSAL
BARCODE READER

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 11:29

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

DIAGNOSTIC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 11:40

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:41
02 Std. Sol.	0.000	11:42
03 Room Air	0.000	11:42
04 Std. Sol.	0.000	11:43
05 Room Air	0.000	11:44
06 Std. Sol.	0.000	11:44
07 Room Air	0.000	11:45

08 Sim Temp = 34.0°C

Simul Ser No = DR3377
Std Sol No = MILLIQ H2O
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: ZERO AC
 0.000 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 11:46

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:47
02 Std. Sol.	0.019	11:48
03 Room Air	0.000	11:48
04 Std. Sol.	0.019	11:49
05 Room Air	0.000	11:50
06 Std. Sol.	0.018	11:50
07 Room Air	0.000	11:51

08 Sim Temp = 34.0°C

Simul Ser No = DR7111
Std Sol No = 17160
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *LOW AC*
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 11:53

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:54
02 Std. Sol.	0.296	11:54
03 Room Air	0.000	11:55
04 Std. Sol.	0.296	11:56
05 Room Air	0.000	11:56
06 Std. Sol.	0.296	11:57
07 Room Air	0.000	11:58

08 Sim Temp = 34.0°C

Simul Ser No = DR3375
Std Sol No = 17350
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: HIGH AC
 0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 11:59

Test	AC	Time
01 Room Air	0.000	12:00
02 *Subject Test	INT*	12:00
03 Room Air	0.000	12:01

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 12:02

Test	AC	Time
01 Room Air	0.000	12:03
02 *Subject Test	INT*	12:03
03 Room Air	0.000	12:04

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.05% ACETONE

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 12:04

Test	AC	Time
01 Room Air	0.000	12:05
02 *Subject Test	INT*	12:06
03 Room Air	0.000	12:06

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666

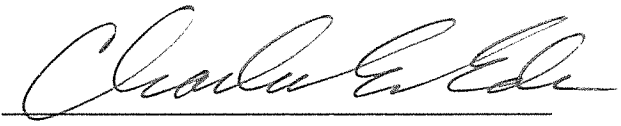

Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10% METHANOL

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 12:06

Test	AC	Time
01 Room Air	0.000	12:08
02 *Subject Test	INT*	12:08
03 Room Air	0.000	12:09

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10% ISOPROPANOL

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 13:34

Test	AC	Time
01 Room Air	AMB*	13:35
02 Room Air	0.000	13:36

*Invalid Test
Check Ambient Conditions

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = AMBIENT FAIL
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *AMBIENT
FAIL*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 13:36

Test	AC	Time
01 Room Air	0.000	13:37
02 Invalid Sample	X.XXX	13:37
03 Room Air	0.000	13:38

*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INVALID SAMPLE
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666

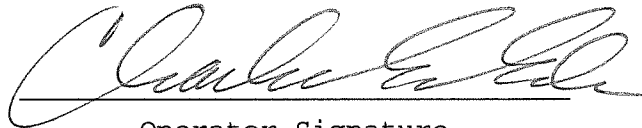

Operator Signature
CHARLES EDER

Remarks: *INVALID
SAMPLE*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 13:38

Test	AC	Time
01 Room Air	0.000	13:39
02 *Subject Test	ABT*	13:39
03 Room Air	0.000	13:40

*Sequence Aborted

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = SEQ ABORT
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: SEQUENCE ABORTED

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 13:43

Test	AC	Time
01 Room Air	0.000	13:44
02 Subject Test 1	0.095	13:44
03 Room Air	0.000	13:45
04 Reported AC	0.095	13:44

No RFI Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = ABA MODE
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666

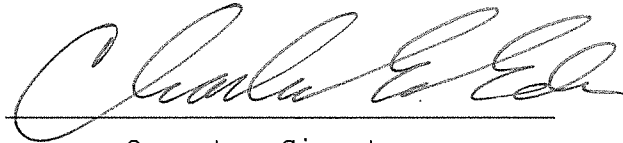

Operator Signature
CHARLES EDER

Remarks:

ABA MODE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 13:46

Test	AC	Time
01 Diagnostic	OK	13:48
02 Room Air	0.000	13:48
03 Subject Test 1	0.095	13:49
04 Room Air	0.000	13:51
05 Std. Gas	0.089*	13:52
06 Room Air	0.000	13:53

*Cal Check Out of Tolerance

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = CAL CHK OUT TOL
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
OUT OF TOLERANCE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 13:57

Test	AC	Time
01 Diagnostic	OK	13:58
02 Room Air	0.000	13:59
03 Subject Test 1	0.094	13:59
04 Room Air	0.000	14:01
05 Std. Gas	0.079	14:02
06 Room Air	0.000	14:04
07 *Subject Test	RFI*	14:04
08 Room Air	0.000	14:04

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI DETECTED
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *RFI DETECTED*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 14:05

Test	AC	Time
01 Diagnostic	OK	14:06
02 Room Air	0.000	14:07
03 *Subject Test	0.000*	14:10
04 Room Air	0.000	14:12
05 Std. Gas	0.080	14:13
06 Room Air	0.000	14:14
07 *Subject Test	0.000*	14:17
08 Room Air	0.000	14:18

No RFI Detected

*Deficient Sample - Value Printed was
Highest Obtained

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = DEFICIENT SAMP
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
CHARLES EDER

Remarks: DEFICIENT
SAMPLES

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 14:20

Test	AC	Time
01 Diagnostic	OK	14:21
02 Room Air	0.000	14:22
03 Reference	IPS*	14:22
04 Room Air	0.000	14:22

*Improper Sample

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = IMPROPER SAMPLE
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

*IMPROPER
SAMPLE*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 14:23

Test	AC	Time
01 Diagnostic	OK	14:24
02 Room Air	0.000	14:24
03 Subject Test 1	0.244*	14:25
04 Room Air	0.000	14:27
05 Std. Gas	0.080	14:28
06 Room Air	0.000	14:29
07 Subject Test 2	0.092*	14:30
08 Room Air	0.000	14:31

*Difference Too Great

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = DIFF TOO GREAT
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *DIFFERENCE
TOO GREAT*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 14:32


Test	AC	Time
01 Diagnostic	OK	14:32
02 Room Air	0.000	14:33
03 Subject Test 1	0.093	14:33
04 Room Air	0.000	14:36
05 Std. Gas	0.079	14:37
06 Room Air	0.000	14:38
07 Subject Test 2	0.093	14:38
08 Room Air	0.000	14:39
09 Reported AC	0.093	14:33

Difference OK
No RFI Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = CMS MODE
Dr. Lic. = ND/DIS821456
Lot No = 17618080A1
Cyl No = 28
Expiration Date = 08/05/2020
County = 08 Oper No. = 666666

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

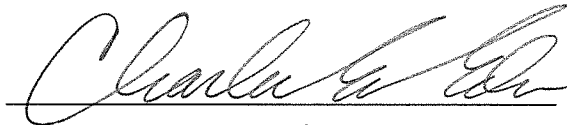

Operator Signature
CHARLES EDER

Remarks: *CMS MODE*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-007091
Location = TOXL 8164.16.00 09/18
11/08/2018 14:40

Test	AC	Time
01 Room Air	0.000	14:40
02 Std. Gas	0.079	14:41
03 Room Air	0.000	14:41
04 Std. Gas	0.078	14:41
05 Room Air	0.000	14:42
06 Std. Gas	0.079	14:42
07 Room Air	0.000	14:43
08 Std. Gas	0.080	14:43
09 Room Air	0.000	14:44
10 Std. Gas	0.080	14:44
11 Room Air	0.000	14:45
12 Std. Gas	0.079	14:45
13 Room Air	0.000	14:45
14 Std. Gas	0.080	14:46
15 Room Air	0.000	14:46
16 Std. Gas	0.080	14:47
17 Room Air	0.000	14:47
18 Std. Gas	0.080	14:48
19 Room Air	0.000	14:48
20 Std. Gas	0.080	14:48
21 Room Air	0.000	14:49
22 Std. Gas	0.079	14:49
23 Room Air	0.000	14:50
24 Std. Gas	0.080	14:50
25 Room Air	0.000	14:51
26 Std. Gas	0.080	14:51
27 Room Air	0.000	14:52
28 Std. Gas	0.080	14:52
29 Room Air	0.000	14:52
30 Std. Gas	0.080	14:53
31 Room Air	0.000	14:53
32 Std. Gas	0.080	14:54
33 Room Air	0.000	14:54
34 Std. Gas	0.080	14:54
35 Room Air	0.000	14:55
36 Std. Gas	0.080	14:55
37 Room Air	0.000	14:56
38 Std. Gas	0.080	14:56
39 Room Air	0.000	14:57
40 Std. Gas	0.081	14:57
41 Room Air	0.000	14:58
42 Cal Check Stats:		
43 Average	0.0798	
44 Std Dev	0.0006	
45 Rel Std Dev	0.81%	



Operator Signature
CHARLES EDER

Remarks: STABILITY TEST

Form 106-I8000

0.080 AC

LOT: 17618080A1

CYL: 028

Exp: 8/5/2020