

### INTOXILYZER® 8000 INITIAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006675

#### A. GENERAL Setup and Checks:

- Power On  
 5 min. countdown during initial warm-up  
 1 min. countdown to begin test after standby mode
- Display Intensity (Ctrl + ↑ or ↓)
- Password Security:  
 Level 1 (Operator)    Level 2 (Field Inspector)    Level 3 (Lab Personnel)
- Printer Setup (Level 3,S,P)
- Forms Load (CMI, Inc., CoBrA Software)

#### B. LEVEL 1 Setup and Checks:

- Internal Printer Test and Paper Feed (Level 1,P). Attach record.
- External Printer Test (Level 1,P). Attach record.
- Barcode Reader (Level 1,B):  
 Operator ID    ND License    R key: Refusal. Attach record.

#### C. LEVEL 2 Setup and Checks:

- Continuous Air Blank (Level 2,A)
- Diagnostic (Level 2,D). Attach record.
- Prelim Data Entry (Level 2,E)
- Ser Number/Version Info (Level 2,V):  
Inst Ser#: 80-006675   DSP Ver: 1362.14  
Core Ver: 8164.14   CPLD Ver: 7

#### D. LEVEL 3 Setup and Checks:

- DVM Monitor (Level 3,D,D): 3: 12482 s: 1 c: 47.00  
9: 12954 s: 1 B: 45 0  
(RFI indicator with keyed radio): 1
- Function (F) Keys: :  F5 – Tone                       F9 - Fan  
 F6 – Green LED                     F10 – Pump  
 F7 – Red LED                         F11 – Solenoid
- Atmospheric Monitor (Level 3,D,A): Atmo Sensor, P: 945 CF: 1.07
- Flow Monitor (Level 3,D,F): Flow Sensor, R: 228 F: 0.000 L/s

5. Temperature Monitor (Level 3,D,T): C: 47.0 A: 48.0 I: 0.0  
B: 45.0 V: 0.0
6. Tank Monitor (Level 3,D,G): P (display): 884 psi P (gauge): ~875 psi
7.  General Setup (Level 3,S,G)
8.  Configure Start Test (Level 3,S,T)
9.  Network (Level 3,S,N)

**E. TESTS (attach all test records):**

**Configure wet bath simulator standards before running tests (Level 1,S):**

1. Zero AC (Level 1,C):  
Sim ser #: MP3064 Lot #: MILLI Q H<sub>2</sub>O Exp date: NA  
Known value: 0.000 AC  
Results: 0.000 AC 0.000 AC 0.000 AC
2. Low AC (Level 1,C):  
Sim ser #: MP3003 Lot #: 201603H Exp date: 3.16.2018  
Known value: 0.010 AC  
Results: 0.010 AC 0.010 AC 0.011 AC
3. High AC (Level 1,C):  
Sim ser #: MP3063 Lot #: 16102 Exp date: 3.22.2018  
Known value: 0.400 AC  
Results: 0.392 AC 0.393 AC 0.393 AC

**Configure dry gas standard before running tests (Level 1,S):**

4. Ethanol + 0.05% Acetone (Level 1,B):  
Sim ser #: DR5135 Lot #: ICS4 Exp date: 9.9.2017  
Known value: 0.10AC + 0.05% ACETONE  
 Display reads "Interferent Detect"
5. Acetone (Level 1,B):  
Sim ser #: DR5143 Lot #: ACE2 Exp date: 9.29.17  
Known value: 0.05% ACETONE  
 Display reads "Interferent Detect"
6. Methanol (Level 1,B):  
Sim ser #: DR3377 Lot #: MET2 Exp date: 9.29.17  
Known value: 0.10% METHANOL  
 Display reads "Interferent Detect"
7. Isopropanol (Level 1,B):  
Sim ser #: DR3453 Lot #: IPA2 Exp date: 9.29.17  
Known value: 0.10% ISOPROPANOL  
 Display reads "Interferent Detect"

- 8.  Ambient Fail (Level 1,B): Display and test record read correct.
- 9.  Invalid Sample (Level 1,B): Display and test record read correct.
- 10.  Sequence Aborted (Level 1,B): Display and test record read correct.
- 11.  ABA (Level 1,B): Test record reads correct.
- 12.  Calibration Check Out of Tolerance (CMS mode): Display and test record read correct.
- 13.  RFI Detected (B,C, or CMS mode): Display and test record read correct.
- 14.  Tank Pressure Below Minimum (CMS mode): Display reads correct.
- 15.  Deficient Samples (CMS mode): Display and test record read correct.
- 16.  Improper Sample (CMS mode): Display and test record read correct.
- 17.  Difference Too Great (CMS mode): Display and test record read correct.
- 18.  CMS (CMS mode): Test record reads correct.
- 19. Stability Test (Level 3,T,S):

Ave: 0.0814 Std Dev: 0.0006 Rel Std Dev: 0.74%

Maintenance/Repairs/Notes: INTERNAL PRINT TEST WAS RE-RUN DUE TO  
TAPE X<sub>1</sub> CEE OBSCURING (FADED) CONTENT OF ORIGINAL PRINT TEST.  
Charles E. Edr 1.24.2017

Instrument is acceptable to be used in the field.

Charles E. Edr  
Charles E. Edr  
Field Inspector's Signature

24 JAN. 2017  
1/18/2017  
Date

Deb Shanaver  
Reviewed by

19 Jan 17 DS  
Date 27 Mar 17



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer  
North Dakota Model 8000 SN 80-006675  
Location = TOXL 8164.14.00 09/16  
01/24/2017 12:55

\*\*\*\*\* Printer Test \*\*\*\*\*

12 char/line  
abcdefghijkl  
ABCDEFGHIJKL

16 char per line  
abcdefghijklmnop  
ABCDEFGHIJKLMN

21 chars per line  
abcdefghijklmnopqrstu  
ABCDEFGHIJKLMNQRSTU

24 characters per line  
abcdefghijklmnopqrstuvw  
ABCDEFGHIJKLMNQRSTUW

32 characters per line  
abcdefghijklmnopqrstuvwxy123456  
ABCDEFGHIJKLMNQRSTUWXYZ123456

42 characters per line  
abcdefghijklmnopqrstuvwxy1234567890abcdef  
ABCDEFGHIJKLMNQRSTUWXYZ1234567890ABCDEF

Current Instrument Setup

Data Entry Mode: Enabled  
Start Test Sequence: DABACABA  
Display Prelim Rslt? Yes  
Display Third Digit? Yes  
Inhib Printer(Y/N)? No  
Display Volume? No  
Disable On Memfull? Yes  
# of Print Copies? 1  
Select Std (D/W/I)? Dry  
Standard Value? 0.080  
Standard Lot #? 09216080A3  
Standard Cyl #? 38  
Standard Expiration? 05/05/2018  
Oper No? 666666

Flow Cal. Date: 08/25/2016  
Slope 701  
Intercept -701324

IR Calibration Date: 08/25/2016  
3um 9um  
-----  
0th Coef(\*100): -8608 -21568  
1st Coef(\*100): 258710 128604  
2nd Coef(\*100): 2478 1279  
H2O adj(mg/l)\*10k): 381 528

\*\*\*\*\* Test End \*\*\*\*\*



Operator Signature  
CHARLES EDER

Remarks: *INTERNAL  
PRINT TEST*

Form 106-18000

*ORIGINAL PRINT TEST HAD  
SOME PRINT OBSCURED (FADED)  
BY TAPE.*

*RE-PRINT*





Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006675  
Location = TOXL      8164.14.00 09/16  
01/18/2017      13:25

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *DIAGNOSTIC*



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006675  
Location = TOXL      8164.14.00 09/16  
01/18/2017      13:31

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:32
02 Std. Sol.	0.000	13:33
03 Room Air	0.000	13:33
04 Std. Sol.	0.000	13:34
05 Room Air	0.000	13:34
06 Std. Sol.	0.000	13:35
07 Room Air	0.000	13:35

08 Sim Temp = 34.0°C

Simul Ser No = MP3064  
Std Sol No = MILLIQ H2O  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*ZERO AC*  
*0.000 AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006675  
Location = TOXL      8164.14.00 09/16  
01/18/2017      13:37

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:38
02 Std. Sol.	0.010	13:39
03 Room Air	0.000	13:39
04 Std. Sol.	0.010	13:40
05 Room Air	0.000	13:40
06 Std. Sol.	0.011	13:41
07 Room Air	0.000	13:42

08 Sim Temp = 34.0°C

Simul Ser No = MP3003  
Std Sol No = 201603H  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *Low AC*  
*0.010 AC*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006675  
Location = TOXL      8164.14.00 09/16  
01/18/2017      13:48

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:49
02 Std. Sol.	0.392	13:49
03 Room Air	0.000	13:50
04 Std. Sol.	0.393	13:51
05 Room Air	0.000	13:51
06 Std. Sol.	0.393	13:52
07 Room Air	0.000	13:52

08 Sim Temp = 34.0°C

Simul Ser No = MP3063  
Std Sol No = 16102  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

HIGH AC  
0.400 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006675  
Location = TOXL                    8164.14.00 09/16  
01/18/2017                            13:54

Test	AC	Time
01 Room Air	0.000	13:55
02 *Subject Test	INT*	13:55
03 Room Air	0.000	13:56

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = 0.10AC+0.05ACE  
Dr. Lic. = ND/DIS821456  
Lot No = 09216080A3  
Cyl No = 38  
Expiration Date = 05/05/2018  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *Interferent*  
*0.10AC + 0.05% ACETONE*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006675  
Location = TOXL                 8164.14.00 09/16  
01/18/2017                        13:57

Test	AC	Time
01 Room Air	0.000	13:58
02 *Subject Test	INT*	13:58
03 Room Air	0.000	13:59

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                     Weight = 150  
Test = DUI                             Cit = 0.05 ACETONE  
Dr. Lic. = ND/DIS821456  
Lot No = 09216080A3  
Cyl No = 38  
Expiration Date = 05/05/2018  
County = 08                             Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*Interferent*  
*0.05% ACETONE*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006675  
Location = TOXL                8164.14.00 09/16  
01/18/2017                        13:59

Test	AC	Time
01 Room Air	0.000	14:00
02 *Subject Test	INT*	14:01
03 Room Air	0.000	14:01

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                Weight = 150  
Test = DUI                        Cit = 0.10 METHANOL  
Dr. Lic. = ND/DIS821456  
Lot No = 09216080A3  
Cyl No = 38  
Expiration Date = 05/05/2018  
County = 08                        Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*Interferent*  
*0.10% METHANOL*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006675  
Location = TOXL                8164.14.00 09/16  
01/18/2017                        14:01

Test	AC	Time
01 Room Air	0.000	14:03
02 *Subject Test	INT*	14:03
03 Room Air	0.000	14:04

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                Weight = 150  
Test = DUI                        Cit = 0.10 IPA  
Dr. Lic. = ND/DIS821456  
Lot No = 09216080A3  
Cyl No = 38  
Expiration Date = 05/05/2018  
County = 08                        Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*Interferent*  
*0.10% ISOPROPANOL*

Form 106-I8000





Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006675  
Location = TOXL                8164.14.00 09/16  
01/18/2017                            14:06

Test	AC	Time
01 Room Air	0.000	14:07
02 Invalid Sample	X.XXX	14:07
03 Room Air	0.000	14:08

\*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = INVALID SAMPLE  
Dr. Lic. = ND/DIS821456  
Lot No = 09216080A3  
Cyl No = 38  
Expiration Date = 05/05/2018  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: *INVALID SAMPLE*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006675  
Location = TOXL      8164.14.00 09/16  
01/18/2017      14:08

Test	AC	Time
01 Room Air	0.000	14:10
02 *Subject Test	ABT*	14:10
03 Room Air	0.000	14:10

\*Sequence Aborted

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female      Weight = 150  
Test = DUI      Cit = SEQUENCE ABORTE  
Dr. Lic. = ND/DIS821456  
Lot No = 09216080A3  
Cyl No = 38  
Expiration Date = 05/05/2018  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: SEQUENCE ABORTED



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006675  
Location = TOXL                    8164.14.00 09/16  
01/18/2017                            14:15

Test	AC	Time
01 Diagnostic	OK	14:16
02 Room Air	0.000	14:16
03 Subject Test 1	0.263	14:17
04 Room Air	0.000	14:19
05 Std. Gas	0.089*	14:20
06 Room Air	0.000	14:21

\*Cal Check Out of Tolerance

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = CAL OUT OF TOL  
Dr. Lic. = ND/DIS821456  
Lot No = 09216080A3  
Cyl No = 38  
Expiration Date = 05/05/2018  
County = 08                            Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
OUT OF TOLERANCE

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006675  
Location = TOXL                    8164.14.00 09/16  
01/18/2017                            14:22

Test	AC	Time
01 Diagnostic	OK	14:23
02 Room Air	0.000	14:24
03 Subject Test 1	0.263	14:24
04 Room Air	0.000	14:27
05 Std. Gas	0.082	14:28
06 Room Air	RFI*	14:28
07 Room Air	0.000	14:29

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = RFI DETECTED  
Dr. Lic. = ND/DIS821456  
Lot No = 09216080A3  
Cyl No = 38  
Expiration Date = 05/05/2018  
County = 08                            Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks: RFI DETECTED

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006675  
Location = TOXL                    8164.14.00 09/16  
01/18/2017                            14:29

Test	AC	Time
01 Diagnostic	OK	14:30
02 Room Air	0.000	14:31
03 *Subject Test	0.000*	14:34
04 Room Air	0.000	14:36
05 Std. Gas	0.081	14:37
06 Room Air	0.000	14:38
07 *Subject Test	0.000*	14:41
08 Room Air	0.000	14:42


No RFI Detected

\*Deficient Sample - Value Printed was  
Highest Obtained

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = DEFICIENT SAMP  
Dr. Lic. = ND/DIS821456  
Lot No = 09216080A3  
Cyl No = 38  
Expiration Date = 05/05/2018  
County = 08                            Oper No. = 666666

20 minute waiting period ascertained? Y  
Clean Mouthpiece used and disposed? Y  
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the  
instructions displayed by the Intoxilyzer  
in conducting this test.

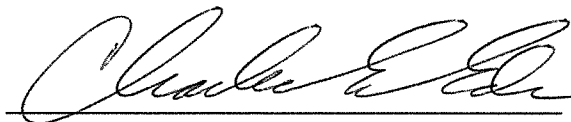

Operator Signature  
CHARLES EDER

Remarks: *DEFICIENT SAMPLES*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006675  
Location = TOXL                 8164.14.00 09/16  
01/18/2017                        14:43

Test	AC	Time
01 Diagnostic	OK	14:44
02 Room Air	0.000	14:44
03 Reference	IPS*	14:45
04 Room Air	0.000	14:45

\*Improper Sample

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = IMPROPER SAMPLE  
Dr. Lic. = ND/DIS821456  
Lot No = 09216080A3  
Cyl No = 38  
Expiration Date = 05/05/2018  
County = 08                            Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

*Improper  
Sample*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006675  
Location = TOXL                    8164.14.00 09/16  
01/18/2017                            14:48

Test	AC	Time
01 Diagnostic	OK	14:49
02 Room Air	0.000	14:50
03 Subject Test 1	0.263*	14:50
04 Room Air	0.000	14:53
05 Std. Gas	0.081	14:54
06 Room Air	0.000	14:55
07 Subject Test 2	0.206*	14:55
08 Room Air	0.000	14:56

\*Difference Too Great

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = DIFF TOO GREAT  
Dr. Lic. = ND/DIS821456  
Lot No = 09216080A3  
Cyl No = 38  
Expiration Date = 05/05/2018  
County = 08                            Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
CHARLES EDER

Remarks: *DIFFERENCE  
TOO GREAT*



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006675  
Location = TOXL                    8164.14.00 09/16  
01/18/2017                            14:57

Test	AC	Time
01 Diagnostic	OK	14:58
02 Room Air	0.000	14:58
03 Subject Test 1	0.261	14:59
04 Room Air	0.000	15:01
05 Std. Gas	0.081	15:02
06 Room Air	0.000	15:04
07 Subject Test 2	0.260	15:04
08 Room Air	0.000	15:05
09 Reported AC	0.260	15:04

Difference OK  
No RFI Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                    Weight = 150  
Test = DUI                            Cit = CMS MODE  
Dr. Lic. = ND/DIS821456  
Lot No = 09216080A3  
Cyl No = 38  
Expiration Date = 05/05/2018  
County = 08                            Oper No. = 666666

20 minute waiting period ascertained? Y  
Clean Mouthpiece used and disposed? Y  
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the  
instructions displayed by the Intoxilyzer  
in conducting this test.



Operator Signature  
CHARLES EDER

Remarks:

CMS MODE

EVIDENTIAL BREATH TEST

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006675  
Location = TOXL      8164.14.00 09/16  
01/18/2017      15:07

Test	AC	Time
01 Room Air	0.000	15:07
02 Std. Gas	0.080	15:07
03 Room Air	0.000	15:08
04 Std. Gas	0.081	15:08
05 Room Air	0.000	15:09
06 Std. Gas	0.082	15:09
07 Room Air	0.000	15:10
08 Std. Gas	0.081	15:10
09 Room Air	0.000	15:11
10 Std. Gas	0.081	15:11
11 Room Air	0.000	15:11
12 Std. Gas	0.082	15:12
13 Room Air	0.000	15:12
14 Std. Gas	0.082	15:13
15 Room Air	0.000	15:13
16 Std. Gas	0.081	15:13
17 Room Air	0.000	15:14
18 Std. Gas	0.082	15:14
19 Room Air	0.000	15:15
20 Std. Gas	0.082	15:15
21 Room Air	0.000	15:16
22 Std. Gas	0.081	15:16
23 Room Air	0.000	15:17
24 Std. Gas	0.082	15:17
25 Room Air	0.000	15:17
26 Std. Gas	0.081	15:18
27 Room Air	0.000	15:18
28 Std. Gas	0.081	15:19
29 Room Air	0.000	15:19
30 Std. Gas	0.081	15:20
31 Room Air	0.000	15:20
32 Std. Gas	0.082	15:20
33 Room Air	0.000	15:21
34 Std. Gas	0.082	15:21
35 Room Air	0.000	15:22
36 Std. Gas	0.082	15:22
37 Room Air	0.000	15:23
38 Std. Gas	0.081	15:23
39 Room Air	0.000	15:24
40 Std. Gas	0.081	15:24
41 Room Air	0.000	15:24
42 Cal Check Stats:		
43 Average	0.0814	
44 Std Dev	0.0006	
45 Rel Std Dev	0.74%	



Operator Signature  
CHARLES EDER

Remarks: STABILITY TEST

Form 106-I8000

LOT: 09216080A3

EXP: 5/5/2018

CYL: 038