

INTOXILYZER® 8000 INITIAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006677

A. GENERAL Setup and Checks:

1. Power On
 - 5 min. countdown during initial warm-up
 - 1 min. countdown to begin test after standby mode
2. Display Intensity (Ctrl + ↑ or ↓)
3. Password Security:
 - Level 1 (Operator) Level 2 (Field Inspector) Level 3 (Lab Personnel)
4. Printer Setup (Level 3,S,P)
5. Forms Load (CMI, Inc., CoBrA Software)

B. LEVEL 1 Setup and Checks:

1. Internal Printer Test and Paper Feed (Level 1,P). Attach record.
2. External Printer Test (Level 1,P). Attach record.
3. Barcode Reader (Level 1,B):
 - Operator ID ND License R key: Refusal. Attach record.

C. LEVEL 2 Setup and Checks:

1. Continuous Air Blank (Level 2,A)
2. Diagnostic (Level 2,D). Attach record.
3. Prelim Data Entry (Level 2,E)
4. Ser Number/Version Info (Level 2,V):
 - Inst Ser#: 80-006677 DSP Ver: 1362-14
 - Core Ver: 8164.14 CPLD Ver: 7

D. LEVEL 3 Setup and Checks:

1. DVM Monitor (Level 3,D,D): 3: 12852 s: 0 c: 47.06
9: 13320 s: 1 B: 44 0
(RFI indicator with keyed radio): 1
2. Function (F) Keys: : F5 – Tone F9 - Fan
 F6 – Green LED F10 – Pump
 F7 – Red LED F11 – Solenoid
3. Atmospheric Monitor (Level 3,D,A): Atmo Sensor, P: 938 CF: 1.07
4. Flow Monitor (Level 3,D,F): Flow Sensor, R: 208 F: 0.000 L/s

5. Temperature Monitor (Level 3,D,T): C: 47.0 A: 49.0 I: 0.0
B: 45.0 V: 0.0
6. Tank Monitor (Level 3,D,G): P (display): 883 psi P (gauge): ~900 psi
7. General Setup (Level 3,S,G)
8. Configure Start Test (Level 3,S,T)
9. Network (Level 3,S,N)

E. TESTS (attach all test records):

Configure wet bath simulator standards before running tests (Level 1,S):

1. Zero AC (Level 1,C):
Sim ser #: MP3064 Lot #: MILLI Q H₂O Exp date: N/A
Known value: 0.000 AC
Results: 0.000 AC 0.000 AC 0.000 AC
2. Low AC (Level 1,C):
Sim ser #: MP3003 Lot #: 2016034 Exp date: 3.16.2018
Known value: 0.010 AC
Results: 0.009 AC 0.009 AC 0.010 AC
3. High AC (Level 1,C):
Sim ser #: MP3063 Lot #: 16102 Exp date: 3.22.2018
Known value: 0.400 AC
Results: 0.397 AC 0.396 AC 0.397 AC

Configure dry gas standard before running tests (Level 1,S):

4. Ethanol + 0.05% Acetone (Level 1,B):
Sim ser #: DR5135 Lot #: ICS4 Exp date: 9.9.2017
Known value: 0.10AC + 0.05% ACETONE
 Display reads "Interferent Detect"
5. Acetone (Level 1,B):
Sim ser #: DR5143 Lot #: ACE2 Exp date: 9.29.17
Known value: 0.05% ACETONE
 Display reads "Interferent Detect"
6. Methanol (Level 1,B):
Sim ser #: DR3377 Lot #: MET2 Exp date: 9.29.17
Known value: 0.10% METHANOL
 Display reads "Interferent Detect"
7. Isopropanol (Level 1,B):
Sim ser #: DR3453 Lot #: IPA2 Exp date: 9.29.17
Known value: 0.10% ISOPROPRANOL
 Display reads "Interferent Detect"

- 8. Ambient Fail (Level 1,B): Display and test record read correct.
- 9. Invalid Sample (Level 1,B): Display and test record read correct.
- 10. Sequence Aborted (Level 1,B): Display and test record read correct.
- 11. ABA (Level 1,B): Test record reads correct.
- 12. Calibration Check Out of Tolerance (CMS mode): Display and test record read correct.
- 13. RFI Detected (B,C, or CMS mode): Display and test record read correct.
- 14. Tank Pressure Below Minimum (CMS mode): Display reads correct.
- 15. Deficient Samples (CMS mode): Display and test record read correct.
- 16. Improper Sample (CMS mode): Display and test record read correct.
- 17. Difference Too Great (CMS mode): Display and test record read correct.
- 18. CMS (CMS mode): Test record reads correct.
- 19. Stability Test (Level 3,T,S):

Ave: 0.0822 Std Dev: 0.0006 Rel Std Dev: 0.72%

Maintenance/Repairs/Notes: INTERNAL PRINT TEST WAS RE-RUN DUE
TO TAPE OBSCURING SOME OF THE ORIGINAL PRINT. CFE 1-24-17
Charles E. Ed 1/24/2017

Instrument is acceptable to be used in the field.

Charles E. Ed
Charles E. Ed
Field Inspector's Signature

1/24/2017
1/20/2017
Date

Deb Shanaver
Reviewed by

27 Mar 17
Date

Intoxilyzer Test Record and Checklist
NDODAG Crime Lab. Div., Bismarck, ND 58501

EMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOWL 8164,14,01 09/16
11/19/2017 15:12

***** Printer Test *****

12 char/line
abcdefghijkl
ABCDEFGHIJKL

16 char per line
abcdefghijklmnop
ABCDEFGHIJKLMN

21 chars per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNQRSTU

24 characters per line
abcdefghijklmnopqrstuwx
ABCDEFGHIJKLMNQRSTUWX

32 characters per line
abcdefghijklmnopqrstuwx123456
ABCDEFGHIJKLMNQRSTUWXYZ123456

42 characters per line
abcdefghijklmnopqrstuwx1234567890abcdef


Start Test Sequence: DABACABA
Display Printout? Yes
Display Third Digit? Yes
Inhib. Interlock? No
Display Volume? No
Display % MenFuel? No
of Print Codes? 1
Select Std (D/W/L)? Dry
Standard Value? 0.100
Standard Lot #? 01
Standard Cyl #? 1004587
Standard Expiration? 11/19/2017
Oper No? 801116

Flow Cal. Date: 08/24/2016
Slope: 696
Intercept: -655673

IR Calibration Date: 08/24/2016

	Sum	Std
0th Coef(*100):	-12424	-22862
1st Coef(*100):	263434	131353
2nd Coef(*100):	5070	1477
H2O adj(mg/l*10K):	569	590

***** Test End *****



Operator Signature
CHARLES EDER

Remarks: INTERNAL
PRINT
TEST
Form 106-18000

Intoxilyzer Test Record and Checklist
NDCAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/24/2017 11:41

***** Printer Test *****

12 char/line
abcdefghijkl
ABCDEFGHIJKL

16 char per line
abcdefghijklmnop
ABCDEFGHIJKLMNPO

21 chars per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNOPQRSTU

24 characters per line
abcdefghijklmnopqrstuvw
ABCDEFGHIJKLMNOPQRSTUWX

32 characters per line
abcdefghijklmnopqrstuvwxy123456
ABCDEFGHIJKLMNOPQRSTUWXYZ123456

42 characters per line
abcdefghijklmnopqrstuvwxy1234567890abcdef
ABCDEFGHIJKLMNOPQRSTUWXYZ1234567890ABCDEF

Current Instrument Setup
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Menfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 09216080A3
Standard Cyl #? 38
Standard Expiration? 05/05/2018
Oper No? 666666

Flow Cal. Date: 08/24/2016
Sicpe 696
Intercept -655873

IR Calibration Date: 08/24/2016
Sun Sun

0th Coef(*100):	-12424	-22862
1st Coef(*100):	263434	131353
2nd Coef(*100):	5070	1477
H2O adj(hg/l*10K):	569	590

***** Test End *****



Operator Signature
CHARLES EDER

Remarks: **INTERNAL
PRINT TEST**

Form 106-18000

**TAPE OBSCURED
ORIGINAL PRINT ON
1ST PRINT TEST**

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 15:16

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-|=|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-|=|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? No
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 80
Standard Cyl #? 1234567
Standard Expiration? 11/11/2017
Oper No? 666666

Flow Cal. Date: 08/24/2016
Slope 696
Intercept -655873

IR Calibration Date: 08/24/2016
 3um 9um

0th Coef(*100): -12424 -22862
1st Coef(*100): 263434 131353
2nd Coef(*100): 5070 1477
H2O adj(mg/l*10k): 569 590

***** Printer Test End *****

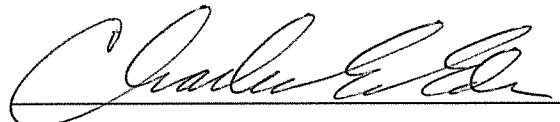

Operator Signature
CHARLES EDER

Remarks: EXTERNAL PRINT
 TEST

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 15:22

Test	AC	Time
01 Room Air	0.000	15:23
02 *Subject Test	REF*	15:23
03 Room Air	0.000	15:24

*Subject Test Refused

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = R KEY REFUSAL
Dr. Lic. = ND/DIS821456
Lot No = 80
Cyl No = 1234567
Expiration Date = 11/11/2017
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: "R" KEY REFUSAL

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 15:25

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *DIAGNOSTIC*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 15:33

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:34
02 Std. Sol.	0.000	15:35
03 Room Air	0.000	15:35
04 Std. Sol.	0.000	15:36
05 Room Air	0.000	15:37
06 Std. Sol.	0.000	15:37
07 Room Air	0.000	15:38

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = MILLIQ H2O
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

ZERO AC
0.000 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 16:06

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:06
02 Std. Sol.	0.009	16:07
03 Room Air	0.000	16:08
04 Std. Sol.	0.009	16:08
05 Room Air	0.000	16:09
06 Std. Sol.	0.010	16:10
07 Room Air	0.000	16:10

08 Sim Temp = 34.0°C

Simul Ser No = MP3003

Std Sol No = 201603H

County = 08

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Low AC

0.010 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 16:13

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:13
02 Std. Sol.	0.397	16:14
03 Room Air	0.000	16:15
04 Std. Sol.	0.396	16:15
05 Room Air	0.000	16:16
06 Std. Sol.	0.397	16:17
07 Room Air	0.000	16:17


08 Sim Temp = 34.0°C

Simul Ser No = MP3063

Std Sol No = 16102

County = 08

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.400 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 16:29

Test	AC	Time
01 Room Air	0.000	16:30
02 *Subject Test	INT*	16:30
03 Room Air	0.000	16:31

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = 0.10AC+0.05ACE
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent
0.10 AC + 0.05% ACETONE


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 16:31

Test	AC	Time
01 Room Air	0.000	16:33
02 *Subject Test	INT*	16:33
03 Room Air	0.000	16:33

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = 0.05 ACETONE
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent
corr 0.10% 0.05% ACETONE


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 16:34

Test	AC	Time
01 Room Air	0.000	16:35
02 *Subject Test	INT*	16:36
03 Room Air	0.000	16:36

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = 0.10 METHANOL
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: 0.10% METHANOL

Interferent

Form 106-18000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 16:36

Test	AC	Time
01 Room Air	0.000	16:37
02 *Subject Test	INT*	16:38
03 Room Air	0.000	16:38

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = 0.10 IPA
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: 0.10% ISOPROPA~~NOL~~

Interferent

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 16:41

Test	AC	Time
01 Room Air	AMB*	16:42
02 Room Air	0.000	16:43

*Invalid Test
Check Ambient Conditions

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = AMBIENT FAIL
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *AMBIENT FAIL*


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 16:43

Test	AC	Time
01 Room Air	0.000	16:44
02 Invalid Sample	X.XXX	16:44
03 Room Air	0.000	16:45

*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INVALID SAMPLE
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *INVALID SAMPLE*


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 16:45

Test	AC	Time
01 Room Air	0.000	16:46
02 *Subject Test	ABT*	16:46
03 Room Air	0.000	16:47

*Sequence Aborted

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = SEQUENCE ABORT
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: SEQUENCE ABORTED

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 16:47

Test	AC	Time
01 Room Air	0.000	16:48
02 Subject Test 1	0.043	16:48
03 Room Air	0.000	16:49
04 Reported AC	0.043	16:48

No RFI Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = ABA MODE
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *ABA MODE*
SINGLE BREATH TEST
Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/19/2017 16:49

Test	AC	Time
01 Diagnostic	OK	16:51
02 Room Air	0.000	16:51
03 Subject Test 1	0.262	16:52
04 Room Air	0.000	16:54
05 Std. Gas	0.090*	16:55
06 Room Air	0.000	16:56

*Cal Check Out of Tolerance

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = CHK OUT OF TOL
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
OUT OF TOLERANCE

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/20/2017 10:08

Test	AC	Time
01 Diagnostic	OK	10:09
02 Room Air	0.000	10:10
03 Subject Test 1	0.257	10:10
04 Room Air	RFI*	10:11
05 Room Air	0.000	10:12

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI DETECTED
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *RFI DETECTED*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/20/2017 10:13

Test	AC	Time
01 Diagnostic	OK	10:14
02 Room Air	0.000	10:14
03 *Subject Test	0.000*	10:17
04 Room Air	0.000	10:19
05 Std. Gas	0.081	10:21
06 Room Air	0.000	10:22
07 *Subject Test	0.000*	10:25
08 Room Air	0.000	10:26
No RFI Detected		

*Deficient Sample - Value Printed was
Highest Obtained

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = DEFICIENT SAMP
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

DEFICIENT
SAMPLES

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/20/2017 10:28

Test	AC	Time
01 Diagnostic	OK	10:29
02 Room Air	IPS*	10:29
03 Room Air	0.000	10:30

*Improper Sample

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = IMPROPER SAMPLE
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *IMPROPER
SAMPLE*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/20/2017 10:30

Test	AC	Time
01 Diagnostic	OK	10:31
02 Room Air	0.000	10:32
03 Subject Test 1	0.258*	10:32
04 Room Air	0.000	10:34
05 Std. Gas	0.082	10:35
06 Room Air	0.000	10:37
07 Subject Test 2	0.205*	10:37
08 Room Air	0.000	10:38

*Difference Too Great

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = DIFF TOO GREAT
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *DIFFERENCE*
TOO GREAT

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/20/2017 10:39


Test	AC	Time
01 Diagnostic	OK	10:39
02 Room Air	0.000	10:40
03 Subject Test 1	0.257	10:40
04 Room Air	0.000	10:43
05 Std. Gas	0.082	10:44
06 Room Air	0.000	10:45
07 Subject Test 2	0.257	10:45
08 Room Air	0.000	10:46
09 Reported AC	0.257	10:45

Difference OK
No RFI Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = CMS MODE
Dr. Lic. = ND/DIS821456
Lot No = 09216080A3
Cyl No = 38
Expiration Date = 05/05/2018
County = 08 Oper No. = 666666

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

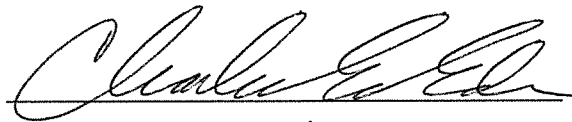

Operator Signature
CHARLES EDER

Remarks: CMS MODE

EVIDENTIAL BREATH TEST

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
01/20/2017 10:47

Test	AC	Time
01 Room Air	0.000	10:47
02 Std. Gas	0.081	10:48
03 Room Air	0.000	10:48
04 Std. Gas	0.082	10:49
05 Room Air	0.000	10:49
06 Std. Gas	0.082	10:49
07 Room Air	0.000	10:50
08 Std. Gas	0.082	10:50
09 Room Air	0.000	10:51
10 Std. Gas	0.082	10:51
11 Room Air	0.000	10:52
12 Std. Gas	0.082	10:52
13 Room Air	0.000	10:53
14 Std. Gas	0.083	10:53
15 Room Air	0.000	10:53
16 Std. Gas	0.082	10:54
17 Room Air	0.000	10:54
18 Std. Gas	0.082	10:55
19 Room Air	0.000	10:55
20 Std. Gas	0.083	10:55
21 Room Air	0.000	10:56
22 Std. Gas	0.083	10:56
23 Room Air	0.000	10:57
24 Std. Gas	0.082	10:57
25 Room Air	0.000	10:58
26 Std. Gas	0.083	10:58
27 Room Air	0.000	10:59
28 Std. Gas	0.082	10:59
29 Room Air	0.000	10:59
30 Std. Gas	0.081	11:00
31 Room Air	0.000	11:00
32 Std. Gas	0.082	11:01
33 Room Air	0.000	11:01
34 Std. Gas	0.082	11:01
35 Room Air	0.000	11:02
36 Std. Gas	0.082	11:02
37 Room Air	0.000	11:03
38 Std. Gas	0.082	11:03
39 Room Air	0.000	11:04
40 Std. Gas	0.083	11:04
41 Room Air	0.000	11:05
42 Cal Check Stats:		
43 Average	0.0822	
44 Std Dev	0.0006	
45 Rel Std Dev	0.72%	



Operator Signature
CHARLES EDER

Remarks:

STABILITY
TEST

Form 106-I8000

Lot: 09216080A3

CYL: 038

Exp: 5/5/2018