

INTOXILYZER® 8000 INITIAL INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006689

A. GENERAL Setup and Checks:

- Power On
 5 min. countdown during initial warm-up
 1 min. countdown to begin test after standby mode
- Display Intensity (Ctrl + ↑ or ↓)
3. Password Security:
 Level 1 (Operator) Level 2 (Field Inspector) Level 3 (Lab Personnel)
- Printer Setup (Level 3,S,P)
- Forms Load (CMI, Inc., CoBrA Software)

B. LEVEL 1 Setup and Checks:

- Internal Printer Test and Paper Feed (Level 1,P). Attach record.
- External Printer Test (Level 1,P). Attach record.
3. Barcode Reader (Level 1,B):
 Operator ID ND License R key: Refusal. Attach record.

C. LEVEL 2 Setup and Checks:

- Continuous Air Blank (Level 2,A)
- Diagnostic (Level 2,D). Attach record.
- Prelim Data Entry (Level 2,E)
4. Ser Number/Version Info (Level 2,V):
Inst Ser#: 80-006689 DSP Ver: 1362.14
Core Ver: 8164.14 CPLD Ver: 7

D. LEVEL 3 Setup and Checks:

1. DVM Monitor (Level 3,D,D): 3: 12682 s: 0 c: 47.00
9: 13160 s: 2 B: 45 0
(RFI indicator with keyed radio): 1
2. Function (F) Keys: : F5 – Tone F9 - Fan
 F6 – Green LED F10 – Pump
 F7 – Red LED F11 – Solenoid
3. Atmospheric Monitor (Level 3,D,A): Atmo Sensor, P: 958 CF: 1.05
4. Flow Monitor (Level 3,D,F): Flow Sensor, R: 231 F: 0.000 L/s

- 5. Temperature Monitor (Level 3,D,T): C: 47.0 A: 48.5 I: 0.0
B: 45.0 V: 0.0 + CE
- 6. Tank Monitor (Level 3,D,G): P (display): 831 psi P (gauge): -825 psi
- 7. General Setup (Level 3,S,G)
- 8. Configure Start Test (Level 3,S,T)
- 9. Network (Level 3,S,N)

E. TESTS (attach all test records):

Configure wet bath simulator standards before running tests (Level 1,S):

- 1. Zero AC (Level 1,C):
Sim ser #: MP3064 Lot #: MILLI Q H₂O Exp date: N/A
Known value: 0.000 AC
Results: 0.000 AC 0.000 AC 0.000 AC
- 2. Low AC (Level 1,C):
Sim ser #: MP3003 Lot #: 2016034 Exp date: 3/16/2018
Known value: 0.010 AC
Results: 0.009 AC 0.009 AC 0.009 AC
- 3. High AC (Level 1,C):
Sim ser #: MP3063 Lot #: 16102 Exp date: 3/22/2018
Known value: 0.400 AC
Results: 0.395 AC 0.395 AC 0.395 AC

Configure dry gas standard before running tests (Level 1,S):

- 4. Ethanol + 0.05% Acetone (Level 1,B):
Sim ser #: DR5135 Lot #: ICS4 Exp date: 9.9.2017
Known value: 0.10 AC + 0.05% ACETONE
 Display reads "Interferent Detect"
- 5. Acetone (Level 1,B):
Sim ser #: DR5143 Lot #: ACE2 Exp date: 9.29.2017
Known value: 0.05% ACETONE
 Display reads "Interferent Detect"
- 6. Methanol (Level 1,B):
Sim ser #: DR3377 Lot #: MET2 Exp date: 9.29.2017
Known value: 0.10% METHANOL
 Display reads "Interferent Detect"
- 7. Isopropanol (Level 1,B):
Sim ser #: DR3453 Lot #: IPA2 Exp date: 9.29.2017
Known value: 0.10% ISOPROPANOL
 Display reads "Interferent Detect"

- 8. Ambient Fail (Level 1,B): Display and test record read correct.
- 9. Invalid Sample (Level 1,B): Display and test record read correct.
- 10. Sequence Aborted (Level 1,B): Display and test record read correct.
- 11. ABA (Level 1,B): Test record reads correct.
- 12. Calibration Check Out of Tolerance (CMS mode): Display and test record read correct.
- 13. RFI Detected (B,C, or CMS mode): Display and test record read correct.
- 14. Tank Pressure Below Minimum (CMS mode): Display reads correct.
- 15. Deficient Samples (CMS mode): Display and test record read correct.
- 16. Improper Sample (CMS mode): Display and test record read correct.
- 17. Difference Too Great (CMS mode): Display and test record read correct.
- 18. CMS (CMS mode): Test record reads correct.

19. Stability Test (Level 3,T,S):


Ave: 0.0820 Std Dev: 0.0006 Rel Std Dev: 0.80%

Maintenance/Repairs/Notes: _____

Instrument is acceptable to be used in the field.


Field Inspector's Signature

26 JAN 2017
Date


Reviewed by

27 Mar 17
Date

Intoxilyzer Test Record and Checklist
NDDAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 12:59

***** Printer Test *****

12 char/line
abcdefghijkl
ABCDEFGHIJKL

16 char per line
abcdefghijklmnop
ABCDEFGHIJKLMN

21 chars per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNQRSTU

24 characters per line
abcdefghijklmnopqrstuvw
ABCDEFGHIJKLMNQRSTUW

32 characters per line
abcdefghijklmnopqrstuvwxy123456
ABCDEFGHIJKLMNQRSTUWXY123456

42 characters per line
abcdefghijklmnopqrstuvwxy1234567890abcdef
ABCDEFGHIJKLMNQRSTUWXY1234567890ABCDEF

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Menfull? No
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.081
Standard Lot #? 81
Standard Cyl #? 11
Standard Expiration? 11/11/2016
Oper No? 666666

Flow Cal. Date: 09/06/2016
Slope: 709
Intercept: -725441

IR Calibration Date: 09/06/2016
3um 9um

0th Coef(*100):	-16013	-23467
1st Coef(*100):	256431	135731
2nd Coef(*100):	2904	1268
H2O adj(mg/l*10K):	553	514

***** Test End *****



Operator Signature
CHARLES EDER

Remarks: *INTERNAL*
PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:02

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? No
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.081
Standard Lot #? 81
Standard Cyl #? 11
Standard Expiration? 11/11/2016
Oper No? 666666

Flow Cal. Date: 09/06/2016
Slope 709
Intercept -725441

IR Calibration Date: 09/06/2016
 3um 9um

	3um	9um
0th Coef(*100):	-16013	-23467
1st Coef(*100):	256431	135731
2nd Coef(*100):	2904	1268
H2O adj(mg/l*10k):	553	514

***** Printer Test End *****

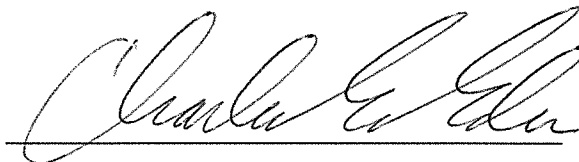

Operator Signature
CHARLES EDER

Remarks:

EXTERNAL
PRINT TEST


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:04

Test	AC	Time
01 Room Air	0.000	13:05
02 *Subject Test	REF*	13:05
03 Room Air	0.000	13:06

*Subject Test Refused

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = R KEY REFUSAL
Dr. Lic. = ND/DIS821456
Lot No = 81
Cyl No = 11
Expiration Date = 11/11/2016
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: "R" KEY REFUSAL

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:09

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *DIAGNOSTIC*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:15

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:16
02 Std. Sol.	0.000	13:17
03 Room Air	0.000	13:17
04 Std. Sol.	0.000	13:18
05 Room Air	0.000	13:18
06 Std. Sol.	0.000	13:19
07 Room Air	0.000	13:19

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = MILLIQ H2O
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

ZERO AC
0.000 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:22

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:23
02 Std. Sol.	0.009	13:25
03 Room Air	0.000	13:25
04 Std. Sol.	0.009	13:26
05 Room Air	0.000	13:27
06 Std. Sol.	0.009	13:27
07 Room Air	0.000	13:28

08 Sim Temp = 34.0°C

Simul Ser No = MP3003
Std Sol No = 201603H
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Low Ac*
 0.010 Ac

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:31

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:32
02 Std. Sol.	0.395	13:33
03 Room Air	0.000	13:33
04 Std. Sol.	0.395	13:34
05 Room Air	0.000	13:34
06 Std. Sol.	0.395	13:35
07 Room Air	0.000	13:36

08 Sim Temp = 34.0°C

Simul Ser No = MP3063
Std Sol No = 16102
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *HIGH AC*
 0.400 AC


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:38

Test	AC	Time
01 Room Air	0.000	13:39
02 *Subject Test	INT*	13:39
03 Room Air	0.000	13:40

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent
0.10 AC + 0.05% ACETONE

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:41

Test	AC	Time
01 Room Air	0.000	13:42
02 *Subject Test	INT*	13:42
03 Room Air	0.000	13:43

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent
0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:44

Test	AC	Time
01 Room Air	0.000	13:44
02 *Subject Test	INT*	13:45
03 Room Air	0.000	13:45

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent
0.10% METHANOL

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:46

Test	AC	Time
01 Room Air	0.000	13:47
02 *Subject Test	INT*	13:48
03 Room Air	0.000	13:48

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666

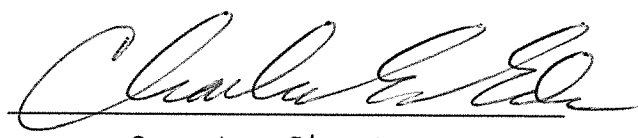

Operator Signature
CHARLES EDER

Remarks:

Interferent
0.10% ISOPROPANOL

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:49

Test	AC	Time
01 Room Air	AMB*	13:50
02 Room Air	0.000	13:51

*Invalid Test
Check Ambient Conditions

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = AMBIENT FAIL
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *AMBIENT
FAIL*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:51

Test	AC	Time
01 Room Air	0.000	13:52
02 Invalid Sample	X.XXX	13:53
03 Room Air	0.000	13:53

*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INVALID SAMPLE
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *INVALID
SAMPLE*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:54

Test	AC	Time
01 Room Air	0.000	13:55
02 *Subject Test	ABT*	13:55
03 Room Air	0.000	13:56

*Sequence Aborted

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = SEQUENCE ABORT
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *SEQUENCE
ABORTED*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 13:56

Test	AC	Time
01 Room Air	0.000	13:57
02 Subject Test 1	0.026	13:57
03 Room Air	0.000	13:58
04 Reported AC	0.026	13:57

No RFI Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = ABA MODE
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

ABA MODE
SINGLE BREATH TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 14:04

Test	AC	Time
01 Diagnostic	OK	14:05
02 Room Air	0.000	14:05
03 Subject Test 1	0.255	14:06
04 Room Air	0.000	14:08
05 Std. Gas	0.089*	14:09
06 Room Air	0.000	14:10

*Cal Check Out of Tolerance

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = CHK OUT OF TOL
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
OUT OF TOLERANCE

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 14:12

Test	AC	Time
01 Diagnostic	OK	14:13
02 Room Air	0.000	14:13
03 *Subject Test	RFI*	14:13
04 Room Air	0.000	14:14

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI DETECTED
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI DETECTED

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 14:14

Test	AC	Time
01 Diagnostic	OK	14:15
02 Room Air	0.000	14:15
03 *Subject Test	0.000*	14:18
04 Room Air	0.000	14:21
05 Std. Gas	0.082	14:22
06 Room Air	0.000	14:23
07 *Subject Test	0.000*	14:26
08 Room Air	0.000	14:27


No RFI Detected

*Deficient Sample - Value Printed was
Highest Obtained

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = DEFICIENT SAMP
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the
instructions displayed by the Intoxilyzer
in conducting this test.

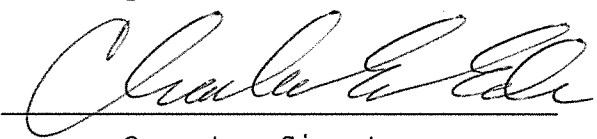

Operator Signature
CHARLES EDER

Remarks: DEFICIENT
SAMPLES

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 14:28

Test	AC	Time
01 Diagnostic	OK	14:29
02 Room Air	0.000	14:29
03 Reference	IPS*	14:29
04 Room Air	0.000	14:30

*Improper Sample

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = IMPROPER SAMPLE
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

*IMPROPER
SAMPLE*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 14:33

Test	AC	Time
01 Diagnostic	OK	14:34
02 Room Air	0.000	14:35
03 Subject Test 1	0.252*	14:35
04 Room Air	0.000	14:37
05 Std. Gas	0.082	14:38
06 Room Air	0.000	14:40
07 Subject Test 2	0.207*	14:40
08 Room Air	0.000	14:41

*Difference Too Great

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = DIFF TOO GREAT
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: DIFFERENCE
 TOO GREAT

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 14:42

Test	AC	Time
01 Diagnostic	OK	14:43
02 Room Air	0.000	14:44
03 Subject Test 1	0.250	14:44
04 Room Air	0.000	14:46
05 Std. Gas	0.081	14:47
06 Room Air	0.000	14:49
07 Subject Test 2	0.247	14:51
08 Room Air	0.000	14:51
09 Reported AC	0.247	14:51

Difference OK
No RFI Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = CMS MODE
Dr. Lic. = ND/DIS821456
Lot No = 17316080A2
Cyl No = 31
Expiration Date = 08/05/2018
County = 08 Oper No. = 666666

20 minute waiting period ascertained? Y
Clean Mouthpiece used and disposed? Y
Clean Mouthpiece used and disposed? Y

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER


Remarks: CMS MODE

EVIDENTIAL BREATH TEST

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006684
Location = TOXL 8164.14.00 09/16
01/26/2017 14:53

Test	AC	Time
01 Room Air	0.000	14:53
02 Std. Gas	0.081	14:54
03 Room Air	0.000	14:54
04 Std. Gas	0.081	14:55
05 Room Air	0.000	14:55
06 Std. Gas	0.081	14:56
07 Room Air	0.000	14:56
08 Std. Gas	0.082	14:56
09 Room Air	0.000	14:57
10 Std. Gas	0.081	14:57
11 Room Air	0.000	14:58
12 Std. Gas	0.083	14:58
13 Room Air	0.000	14:59
14 Std. Gas	0.082	14:59
15 Room Air	0.000	15:00
16 Std. Gas	0.082	15:00
17 Room Air	0.000	15:00
18 Std. Gas	0.082	15:01
19 Room Air	0.000	15:01
20 Std. Gas	0.082	15:02
21 Room Air	0.000	15:02
22 Std. Gas	0.082	15:02
23 Room Air	0.000	15:03
24 Std. Gas	0.083	15:03
25 Room Air	0.000	15:04
26 Std. Gas	0.083	15:04
27 Room Air	0.000	15:05
28 Std. Gas	0.082	15:05
29 Room Air	0.000	15:06
30 Std. Gas	0.083	15:06
31 Room Air	0.000	15:06
32 Std. Gas	0.082	15:07
33 Room Air	0.000	15:07
34 Std. Gas	0.082	15:08
35 Room Air	0.000	15:08
36 Std. Gas	0.082	15:09
37 Room Air	0.000	15:09
38 Std. Gas	0.082	15:09
39 Room Air	0.000	15:10
40 Std. Gas	0.082	15:10
41 Room Air	0.000	15:11
42 Cal Check Stats:		
43 Average	0.0820	
44 Std Dev	0.0006	
45 Rel Std Dev	0.80%	

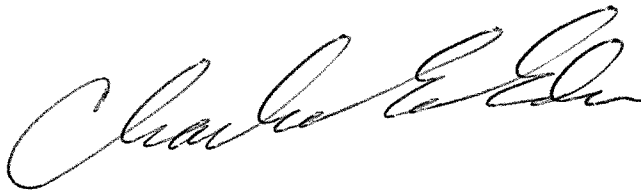

Operator Signature
CHARLES EDER

Remarks:

STABILITY^Y CEE
TEST

Form 106-I8000

LOT: 17316080A2

CYL: 031

EXP: 8/5/2018