




# INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59281 (10-2016)

|  |                               |
|--|-------------------------------|
| Serial Number  | Instrument Location           |
| 80-006690  | RUGB - (NACTC Breaking Rugby) |
| Reason for Install/Repair  |                               |
| <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change<br><input type="checkbox"/> Other (Specify) _____ |                               |

### Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level 1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if Any): \_\_\_\_\_
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature 

Date 05/09/2017

### Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified by Deb Shanaver

Certified Date 10 May 17

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006690  
Location = RUGB                    8164.14.00 09/16  
05/09/2017                            23:34

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-=  
|  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&^\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-=  
|  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%&^\*()\_+?

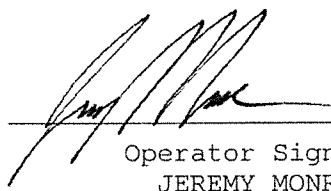
Current Instrument Setup

Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?         1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            09216080A3  
Standard Cyl #?            33  
Standard Expiration?       05/05/2018  
Oper No?                    129922  
  
Flow Cal. Date:            09/07/2016  
Slope                      692  
Intercept                  -621180

IR Calibration Date:       09/07/2016

|                    | 3um    | 9um    |
|--------------------|--------|--------|
| 0th Coef(*100):    | -16902 | -23561 |
| 1st Coef(*100):    | 276538 | 132171 |
| 2nd Coef(*100):    | 1702   | 1220   |
| H2O adj(mg/l*10k): | 497    | 526    |

\*\*\*\*\* Printer Test End \*\*\*\*\*

  
\_\_\_\_\_  
Operator Signature  
JEREMY MONROE

Remarks:

Print Test

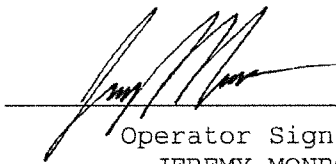
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006690  
Location = RUGB      8164.14.00 09/16  
05/09/2017      23:34

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 23:35 |
| 02 Std. Gas | 0.081 | 23:35 |
| 03 Room Air | 0.000 | 23:36 |
| 04 Std. Gas | 0.080 | 23:36 |
| 05 Room Air | 0.000 | 23:37 |
| 06 Std. Gas | 0.081 | 23:37 |
| 07 Room Air | 0.000 | 23:38 |

Lot No = 09216080A3  
Cyl No = 33  
Exp Date = 05/05/2018  
County = 35      Oper No. = 129922

  
\_\_\_\_\_  
Operator Signature  
JEREMY MONROE

Remarks:

ACA Test

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006690  
Location = RUGB      8164.14.00 09/16  
05/09/2017      23:40

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | RFI*  | 23:41 |
| 02 Room Air | 0.000 | 23:42 |

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, SUBJECT NA  
Sub DOB = 11/29/1987  
Sub Sex = Male      Weight = 135  
Test = DUI      Cit = NA  
Dr. Lic. = ND/NA  
Lot No = 09216080A3  
Cyl No = 33  
Expiration Date = 05/05/2018  
County = 35      Oper No. = 129922

  
Operator Signature  
JEREMY MONROE

Remarks:

*RFI Test*

Form 106-I8000