



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59281 (10-2016)

Serial Number <i>80-000689</i>	Instrument Location <i>EMMONS Sheriff's Office</i>
Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if Any): _____
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

NA
 none performed
 14 Dec 17
 BSN

Field Inspector Signature <i>[Signature]</i>	Date <i>12/13/17</i>
---	-------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified by <i>Roberta Huegel - Nimmo</i>	Certified Date <i>12/14/17</i>
--	-----------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = LINT 8164.14.00 09/16
12/13/2017 14:59

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 19817080A4
Standard Cyl #? 1
Standard Expiration? 09/05/2019
Oper No? 130117

Flow Cal. Date: 09/19/2017
Slope 625
Intercept -591019

IR Calibration Date: 09/19/2017

	3um	9um
0th Coef(*100):	-14072	-18220
1st Coef(*100):	273930	133081
2nd Coef(*100):	2533	1211
H2O adj(mg/l*10k):	588	599

***** Printer Test End *****

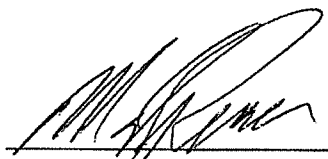

Operator Signature
MARK PEARSON

Remarks:

Initial Test


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = LINT 8164.14.00 09/16
12/13/2017 15:02

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:02
02 Std. Gas	0.083	15:03
03 Room Air	0.000	15:03
04 Std. Gas	0.083	15:04
05 Room Air	0.000	15:04
06 Std. Gas	0.083	15:05
07 Room Air	0.000	15:05

Lot No = 19817080A4
Cyl No = 1
Exp Date = 09/05/2019
County = 15 Oper. No. = 130117

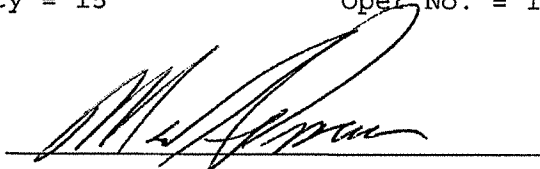
Operator Signature
MARK PEARSON

Remarks:

Form 106-I8000

Instal

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006689
Location = LINT 8164.14.00 09/16
12/13/2017 15:00

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:00
02 Std. Gas	0.082	15:01
03 Room Air	RFI*	15:01
04 Room Air	0.000	15:01

*Invalid Test
Inhibited - RFI

Lot No = 19817080A4
Cyl No = 1
Exp Date = 09/05/2019
County = 15 Oper No. = 130117

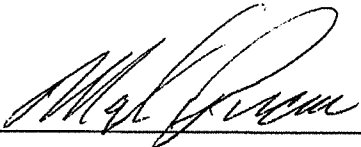

Operator Signature
MARK PEARSON

Remarks:

Form 106-I8000
RFI Test 10/5/17