



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59281 (10-2016)

Serial Number 80-006673	Instrument Location WCPO 1201 12th ST STE Mckenzie County Correctional facility Sully port
Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if Any): N/A
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <i>Ofc. John A. 1143</i>	Date 3-7-18
---	-----------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified by <i>Roberta Hugo-Ninno</i>	Certified Date 3-9-18
--	---------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006673
Location = WCPD 8164.14.00 09/16
03/07/2018 15:59

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

Current Instrument Setup

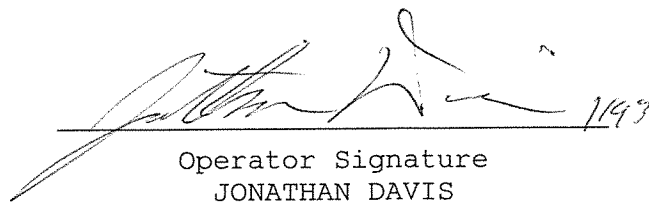
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 03417080A3
Standard Cyl #? 29
Standard Expiration? 03/05/2019
Oper No? 131748

Flow Cal. Date: 03/30/2017
Slope 697
Intercept -667725

IR Calibration Date: 03/30/2017
3um 9um

0th Coef(*100): -9136 -17613
1st Coef(*100): 267126 133333
2nd Coef(*100): 5438 1698
H2O adj(mg/l*10k): 684 589

***** Printer Test End *****


Operator Signature
JONATHAN DAVIS

Remarks:

Install

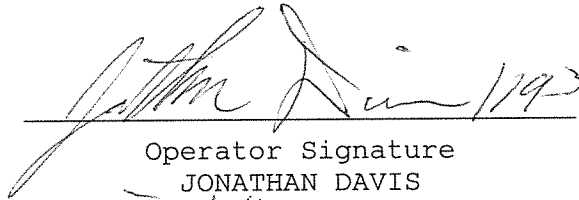
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006673
Location = WCPD 8164.14.00 09/16
03/07/2018 16:00

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:00
02 Std. Gas	0.082	16:01
03 Room Air	0.000	16:01
04 Std. Gas	0.080	16:02
05 Room Air	0.000	16:02
06 Std. Gas	0.081	16:02
07 Room Air	0.000	16:03

Lot No = 03417080A3
Cyl No = 29
Exp Date = 03/05/2019
County = 27 Oper No. = 131748


Operator Signature
JONATHAN DAVIS

Remarks: *Install*

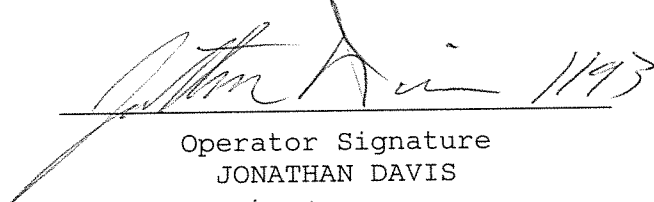
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006673
Location = WCPD 8164.14.00 09/16
03/07/2018 16:04

Test	AC	Time
01 Room Air	0.000	16:05
02 *Subject Test	RFI*	16:05
03 Room Air	0.000	16:06

*Invalid Test
Inhibited - RFI

Sub Name = INSTALL, INSTALL I
Sub DOB = 01/01/1990
Sub Sex = Male Weight = NA
Test = DUI Cit = NA
Dr. Lic. = ND/INSTALL
Lot No = 03417080A3
Cyl No = 29
Expiration Date = 03/05/2019
County = 27 Oper No. = 131748


Operator Signature
JONATHAN DAVIS

Remarks: *Install*