



**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**  
 OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION  
 Toxicology Section/Breath Alcohol Program  
 SFN 59281 (10-2016)

Serial Number <b>80-006668</b>	Instrument Location <b>Cass County Jail - Booking</b>
Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level 1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if Any): none
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <b>Robert Allen</b>	# <b>090801</b>	Date <b>4-12-2018</b>
--	-----------------	--------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified by <b>Roberta Huger-Numms</b>	Certified Date <b>4-17-2018</b>
---	------------------------------------



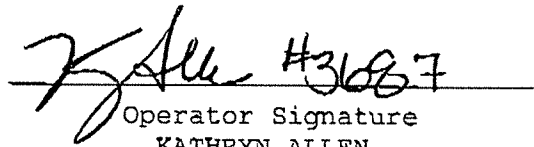
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006668  
Location = CASS      8164.14.00 09/16  
04/12/2018      18:25

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	18:25
02 Std. Gas	0.080	18:26
03 Room Air	0.000	18:26
04 Std. Gas	0.080	18:26
05 Room Air	0.000	18:27
06 Std. Gas	0.081	18:27
07 Room Air	0.000	18:28

Lot No = 19817080A4  
Cyl No = 16  
Exp Date = 09/05/2019  
County = 09      Oper No. = 090801

  
Operator Signature  
KATHRYN ALLEN

Remarks:

Form 106-18000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006668  
Location = CASS      8164.14.00 09/16  
04/12/2018      18:29

Test	AC	Time
01 Room Air	RFI*	18:32
02 Room Air	0.000	18:32

\*Invalid Test  
Inhibited - RFI

Sub Name = INSTAL, RFI TESTING NA  
Sub DOB = 04/11/2018  
Sub Sex = Unknown      Weight = NA  
Test = OTH      Cit = NA  
Dr. Lic. = ND/NA  
Lot No = 19817080A4  
Cyl No = 16  
Expiration Date = 09/05/2019  
County = 09      Oper No. = 090801

 #3667

Operator Signature  
KATHRYN ALLEN

Remarks:

Form 106-I8000