




**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**  
 OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION  
 Toxicology Section/Breath Alcohol Program  
 SFN 59281 (10-2016)

Serial Number	Instrument Location
80-006687	RUGB
Reason for Install/Repair	
<input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:


- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level 1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if Any): \_\_\_\_\_
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

NA  
 7/17/18

Field Inspector Signature	 129922	Date	07/12/2018
---------------------------	--	------	------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified by		Certified Date	07/17/2018
-----------------------	---	----------------	------------

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006687  
Location = RUGB                    8164.14.00 09/16  
07/12/2018                            23:24


DRY CAL CHECK

Test	AC	Time
01 Room Air	RFI*	23:25
02 Room Air	RFI*	23:25

\*Invalid Test  
Inhibited - RFI

Lot No = 34917080A3  
Cyl No = 5  
Exp Date = 02/05/2020  
County = 35                            Oper No. = 129922

  
Operator Signature  
JEREMY MONROE

Remarks:  
  
Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006687  
Location = RUGB      8164.14.00 09/16  
07/12/2018      23:18

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	23:19
02 Std. Gas	0.079	23:19
03 Room Air	0.000	23:19
04 Std. Gas	0.079	23:20
05 Room Air	0.000	23:20
06 Std. Gas	0.079	23:21
07 Room Air	0.000	23:21

Lot No = 34917080A3  
Cyl No = 5  
Exp Date = 02/05/2020  
County = 35      Oper No. = 129922

  
Operator Signature  
JEREMY MONROE

Remarks:  
*New Install*  
Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006687  
Location = RUGB      8164.14.00 09/16  
07/12/2018      23:17

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^&\*()\_+?

Current Instrument Setup

Data Entry Mode: Enabled  
Start Test Sequence: DABACABA  
Display Prelim Rslt? Yes  
Display Third Digit? Yes  
Inhib Printer(Y/N)? No  
Display Volume? No  
Disable On Memfull? Yes  
# of Print Copies? 1  
Select Std (D/W/I)? Dry  
Standard Value? 0.080  
Standard Lot #? 34917080A3  
Standard Cyl #? 5  
Standard Expiration? 02/05/2020  
Oper No? 129922

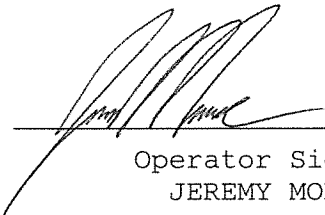
Flow Cal. Date: 05/22/2018  
Slope 624  
Intercept -539297

IR Calibration Date: 05/22/2018

	3um	9um
--	-----	-----

0th Coef(*100):	-22281	-22723
1st Coef(*100):	270132	139077
2nd Coef(*100):	3128	1287
H2O adj (mg/l*10k):	382	400

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
JEREMY MONROE

Remarks:  
New Install