



**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**  
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM  
 SFN 59281 (06/2018)

Serial Number	80-006507	Instrument Location	Grand Forks County Corrections
Reason for Install/Repair			
<input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____			

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level 1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): Yearly inspection at ND State Lab
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature	<i>David Stromberg</i>	Date	05/08/2020
---------------------------	------------------------	------	------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By	<i>Charles E. Ed</i>	Certified Date	5/8/2020
-----------------------	----------------------	----------------	----------

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006507  
Location = GFCC      8164.14.00 09/16  
05/08/2020      13:29

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&\*()\_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&\*()\_+?

Current Instrument Setup

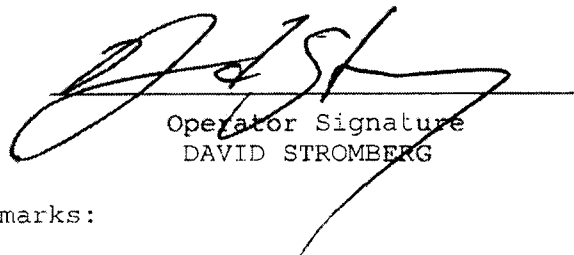
Data Entry Mode:      Enabled  
Start Test Sequence:      DABACABA  
Display Prelim Rslt?      Yes  
Display Third Digit?      Yes  
Inhib Printer(Y/N)?      No  
Display Volume?      No  
Disable On Memfull?      Yes  
# of Print Copies?      1  
Select Std (D/W/I)?      Dry  
Standard Value?      0.080  
Standard Lot #?      24119080A1  
Standard Cyl #?      36  
Standard Expiration?      11/05/2021  
Oper No?      020836

Flow Cal. Date:      08/20/2015  
Slope      659  
Intercept      -658315

IR Calibration Date:      08/20/2015

	3um	9um
0th Coef(*100):	-9452	-11722
1st Coef(*100):	258808	139588
2nd Coef(*100):	4476	1674
H2O adj(mg/l*10k):	499	376

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
DAVID STROMBERG

Remarks:

Form 106-I8000

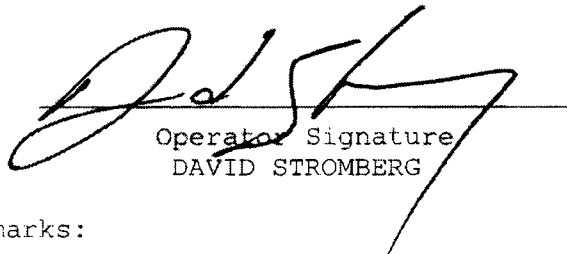
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006507  
Location = GFCC      8164.14.00 09/16  
05/08/2020      13:30

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:30
02 Std. Gas	0.080	13:31
03 Room Air	0.000	13:31
04 Std. Gas	0.081	13:32
05 Room Air	0.000	13:32
06 Std. Gas	0.080	13:33
07 Room Air	0.000	13:33

Lot No = 24119080A1  
Cyl No = 36  
Exp Date = 11/05/2021  
County = 18      Oper No. = 020836

  
Operator Signature  
DAVID STROMBERG

Remarks:

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

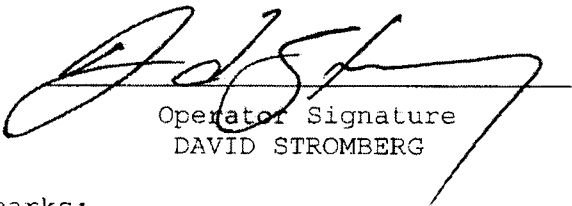
CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006507  
Location = GFCC                    8164.14.00 09/16  
05/08/2020                            13:34

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:34
02 Std. Gas	0.081	13:35
03 Room Air	0.000	13:35
04 Reference	RFI*	13:35
05 Room Air	0.000	13:36

\*Invalid Test  
  Inhibited - RFI

Lot No = 24119080A1  
Cyl No = 36  
Exp Date = 11/05/2021  
County = 18                            Oper No. = 020836

  
Operator Signature  
DAVID STROMBERG

Remarks:

Form 106-I8000