

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006677

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 942 psi Regulator: 950 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3061 Lot #: 201810D Exp. Date: 10.24.20
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP3069 Lot #: 201902D Exp. Date: 2.20.21

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3451 Lot #: JCS 6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 05620 080 A1 Cyl #: 34 Exp. Date: 4.5.22

Test 1	<u>0.081</u>	Test 4	<u>0.081</u>	Test 7	<u>0.081</u>
Test 2	<u>0.081</u>	Test 5	<u>0.082</u>	Test 8	<u>0.082</u>
Test 3	<u>0.081</u>	Test 6	<u>0.081</u>	Test 9	<u>0.081</u>
Average	<u>0.081</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Ed
Breath Analyst Signature

6.10.20
Date

NA

NA

Reviewed by _____

Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
06/10/2020 11:30

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=-|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=-|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 05620080A1
Standard Cyl #? 34
Standard Expiration? 04/05/2022
Oper No? 666666

Flow Cal. Date: 08/24/2016
Slope 696
Intercept -655873

IR Calibration Date: 08/24/2016
 3um 9um

0th Coef(*100): -12424 -22862
1st Coef(*100): 263434 131353
2nd Coef(*100): 5070 1477
H2O adj(mg/l*10k): 569 590

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
06/10/2020 11:35

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:36
02 Std. Sol.	0.017	11:36
03 Room Air	0.000	11:37
04 Std. Sol.	0.018	11:38
05 Room Air	0.000	11:38
06 Std. Sol.	0.018	11:39
07 Room Air	0.000	11:39

08 Sim Temp = 34.0°C

Simul Ser No = MP3061
Std Sol No = 201810D
County = 08 Oper No. = 666666

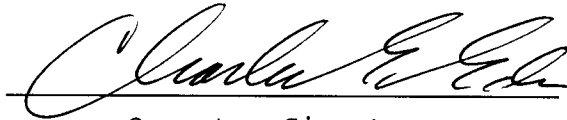

Operator Signature
CHARLES EDER

Remarks:

Low AC

0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
06/10/2020 11:46

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:46
02 Std. Sol.	0.292	11:47
03 Room Air	0.000	11:48
04 Std. Sol.	0.294	11:49
05 Room Air	0.000	11:49
06 Std. Sol.	0.294	11:50
07 Room Air	0.000	11:50

08 Sim Temp = 34.0°C

Simul Ser No = MP3069

Std Sol No = 201902D

County = 08

Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
06/10/2020 11:55

Test	AC	Time
01 Room Air	0.000	11:56
02 *Subject Test	INT*	11:56
03 Room Air	0.000	11:57

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS921456
Lot No = 05620080A1
Cyl No = 34
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666

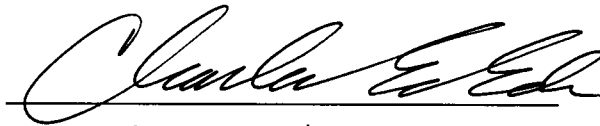

Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10 AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
06/10/2020 11:57

Test	AC	Time
01 Diagnostic	OK	11:58
02 Room Air	0.000	11:58
03 *Subject Test	RFI*	11:58
04 Room Air	0.000	11:59

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS921456
Lot No = 05620080A1
Cyl No = 34
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *RFI CHECK*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
06/10/2020 11:59

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:00
02 Std. Gas	0.081	12:00
03 Room Air	0.000	12:00
04 Std. Gas	0.081	12:01
05 Room Air	0.000	12:01
06 Std. Gas	0.081	12:02
07 Room Air	0.000	12:02

Lot No = 05620080A1
Cyl No = 34
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

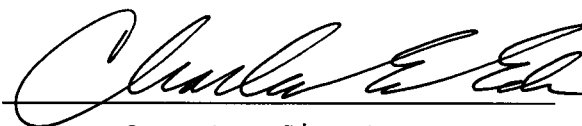

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
06/10/2020 12:02

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:03
02 Std. Gas	0.081	12:03
03 Room Air	0.000	12:04
04 Std. Gas	0.082	12:04
05 Room Air	0.000	12:05
06 Std. Gas	0.081	12:05
07 Room Air	0.000	12:05

Lot No = 05620080A1
Cyl No = 34
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

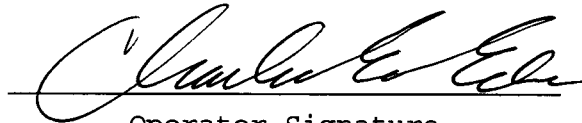

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006677
Location = TOXL 8164.14.00 09/16
06/10/2020 12:06

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:06
02 Std. Gas	0.081	12:07
03 Room Air	0.000	12:07
04 Std. Gas	0.082	12:08
05 Room Air	0.000	12:08
06 Std. Gas	0.081	12:08
07 Room Air	0.000	12:09

Lot No = 05620080A1
Cyl No = 34
Exp Date = 04/05/2022
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000