



**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**  
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM  
 SFN 59281 (06/2018)

Serial Number	80-006690	Instrument Location	Minot AFB, 58703
Reason for Install/Repair			
<input type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) <u>Annual install</u>			

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level 1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): N/A
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature		Date	25 JUNE 2020
---------------------------	--	------	--------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By		Certified Date	6.26.2020
-----------------------	--	----------------	-----------

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006690  
Location = MNAF                    8164.14.00 09/16  
06/25/2020                            15:13

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&\*()\_+?

Current Instrument Setup

Data Entry Mode:                    Enabled  
Start Test Sequence:                DABACABA  
Display Prelim Rslt?                Yes  
Display Third Digit?                Yes  
Inhib Printer(Y/N)?                No  
Display Volume?                    No  
Disable On Memfull?                Yes  
# of Print Copies?                  1  
Select Std (D/W/I)?                Dry  
Standard Value?                    0.080  
Standard Lot #?                    34418080A2  
Standard Cyl #?                    6  
Standard Expiration?                02/05/2021  
Oper No?                            132688

Flow Cal. Date:                    08/23/2018  
Slope                                677  
Intercept                            -593298

IR Calibration Date:                08/23/2018

	3um	9um
0th Coef(*100):	-8380	-21663
1st Coef(*100):	265142	130429
2nd Coef(*100):	3933	1429
H2O adj(mg/l*10k):	412	539

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
DESMOND CALHOUN

Remarks:

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006690  
Location = MNAF      8164.14.00 09/16  
06/25/2020      15:33

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:34
02 Std. Gas	0.078	15:34
03 Room Air	0.000	15:34
04 Std. Gas	0.079	15:35
05 Room Air	0.000	15:35
06 Std. Gas	0.078	15:36
07 Room Air	0.000	15:36

Lot No = 34418080A2  
Cyl No = 6  
Exp Date = 02/05/2021  
County = 64      Oper No. = 132688

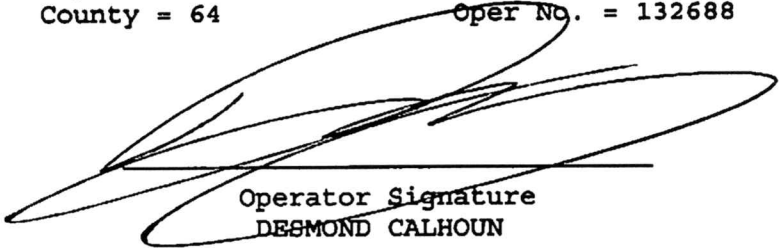

Operator Signature  
DESMOND CALHOUN

Remarks:

Form 106-I8000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006690  
Location = MNAF      8164.14.00 09/16  
06/25/2020      15:24

Test	AC	Time
01 Room Air	0.000	15:25
02 Subject Test 1	0.000	15:26
03 Room Air	RFI*	15:26
04 Room Air	RFI*	15:26

\*Invalid Test  
Inhibited - RFI

Sub Name = CALHOUN, DESMOND HENTON  
Sub DOB = 06/21/1998  
Sub Sex = Male      Weight = 170  
Test = DUI      Cit = 64  
Dr. Lic. = ND/CAL987966  
Lot No = 34418080A2  
Cyl No = 6  
Expiration Date = 02/05/2021  
County = 64      Oper No. = 132688

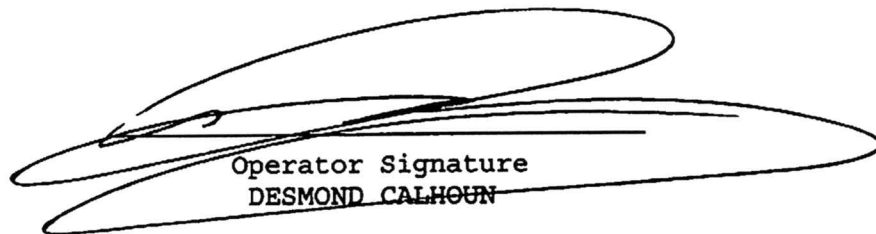

Operator Signature  
DESMOND CALHOUN

Remarks:

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006690  
Location = MNAF      8164.14.00 09/16  
06/25/2020      15:28

Test	AC	Time
01 Room Air	0.000	15:29
02 Subject Test 1	0.000	15:30
03 Room Air	0.000	15:30
04 Reported AC	0.000	15:30

No RFI Detected

Sub Name = MOORE, ERIC G  
Sub DOB = 10/11/1997  
Sub Sex = Male      Weight = 140  
Test = DUI      Cit = NA  
Dr. Lic. = ND/NA  
Lot No = 34418080A2  
Cyl No = 6  
Expiration Date = 02/05/2021  
County = 64      Oper No. = 132688



Operator Signature  
DESMOND CALHOUN

Remarks:

Form 106-I8000