



**ETHANOL GAS STANDARD CYLINDER REPORT**  
 OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION  
 Toxicology Section/Breath Alcohol Program  
 SFN 59282 (10-2013)

Chemical Test Operator Name (Print) <i>Hakonen, Jacquelyn</i>		
Location <i>NTPD</i>	Intoxilyzer® Serial Number <i>80-006672</i>	
Gas Lot Number <i>24119080A1</i>	Gas Cylinder Number <i>10</i>	Gas Expiration Date <i>11/5/2021</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).  
 Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
  - A. *0.082* AC
  - B. *0.082* AC
  - C. *0.083* AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
  - A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).
  - B. ACA Test Record.

Chemical Test Operator Signature <i>Jacquelyn Hakonen</i>	Date <i>February 18, 2021</i>
Reviewed By (Crime Laboratory Use Only) <i>[Signature]</i>	Date <i>2.19.2021</i>


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006672  
Location = NTPD      8164.14.00 09/16  
02/18/2021      11:57

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:58
02 Std. Gas	0.082	11:58
03 Room Air	0.000	11:59
04 Std. Gas	0.082	11:59
05 Room Air	0.000	12:00
06 Std. Gas	0.083	12:00
07 Room Air	0.000	12:01

Lot No = 24119080A1  
Cyl No = 10  
Exp Date = 11/05/2021  
County = 31      Oper No. = 130826

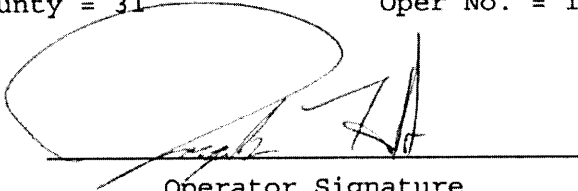

Operator Signature  
JACQUELYN HALONEN

Remarks:

Replaced Expired std. gas

Form 106-18000