



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59281 (06/2018)

Serial Number 80-006691	Instrument Location Kenmare Police Dept.
Reason for Install/Repair	
<input type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input checked="" type="checkbox"/> Other (Specify) New Gas Cylinder Installation	

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): Gas Cylinder Installation
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature 	Date 4/10/2021
-------------------------------	--------------------------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By 	Certified Date 4.23.2021
---------------------------	------------------------------------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006691
Location = KMPD 8164.14.00 09/16
04/10/2021 20:26

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 02621080A1
Standard Cyl #? 030
Standard Expiration? 03/05/2023
Oper No? 132664

Flow Cal. Date: 08/28/2018
Slope 699
Intercept -660610

IR Calibration Date: 08/28/2018

	3um	9um
0th Coef(*100):	-9426	-20764
1st Coef(*100):	258193	134855
2nd Coef(*100):	3532	1465
H2O adj(mg/l*10k):	408	547

***** Printer Test End *****



Operator Signature
CHRISTOPHER ALMLIE

Remarks:


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006691
Location = KMPD 8164.14.00 09/16
04/10/2021 20:26

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	20:27
02 Std. Gas	0.082	20:27
03 Room Air	0.000	20:28
04 Std. Gas	0.082	20:28
05 Room Air	0.000	20:29
06 Std. Gas	0.082	20:29
07 Room Air	0.000	20:29

Lot No = 02621080A1
Cyl No = 030
Exp Date = 03/05/2023
County = 51 Oper No. = 132664


Operator Signature
CHRISTOPHER ALMLIE

Remarks:

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006691
Location = KMPD 8164.14.00 09/16
04/10/2021 20:30

Test	AC	Time
01 Room Air	RFI*	20:31
02 Room Air	0.000	20:32

*Invalid Test
Inhibited - RFI

Sub Name = TEST, TEST TEST
Sub DOB = 04/10/1991
Sub Sex = Unknown Weight = NA
Test = OTH Cit = NA
Dr. Lic. = ND/NA
Lot No = 02621080A1
Cyl No = 030
Expiration Date = 03/05/2023
County = 51 Oper No. = 132664

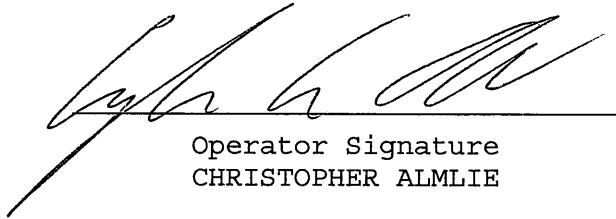

Operator Signature
CHRISTOPHER ALMLIE

Remarks:

Form 106-I8000