

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006673 Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 957 psi Regulator: 950 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: IC56 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621080A1 Cyl #: 25 Exp. Date: 3.5.2023

Test 1 <u>0.082</u>	Test 4 <u>0.082</u>	Test 7 <u>0.082</u>
Test 2 <u>0.082</u>	Test 5 <u>0.082</u>	Test 8 <u>0.081</u>
Test 3 <u>0.082</u>	Test 6 <u>0.082</u>	Test 9 <u>0.081</u>
Average <u>0.082</u>		

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles L. Diet
Breath Analyst Signature

5/5/2021
Date

Kali L. Diet
Reviewed by

9-11-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006673
Location = TOXL 8164.14.00 09/16
05/05/2021 10:29

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 05620080A1
Standard Cyl #? 33
Standard Expiration? 04/05/2022
Oper No? 666666

Flow Cal. Date: 03/30/2017
Slope 697
Intercept -667725

IR Calibration Date: 03/30/2017

	3um	9um
0th Coef (*100):	-9136	-17613
1st Coef (*100):	267126	133333
2nd Coef (*100):	5438	1698
H2O adj (mg/l*10k):	684	589

***** Printer Test End *****


Operator Signature
CHARLES EDER

Remarks: PRINT TEST

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006673
Location = TOXL 8164.14.00 09/16
05/05/2021 11:02

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:02
02 Std. Sol.	0.017	11:03
03 Room Air	0.000	11:04
04 Std. Sol.	0.017	11:04
05 Room Air	0.000	11:05
06 Std. Sol.	0.018	11:06
07 Room Air	0.000	11:06

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Low AC*
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006673
Location = TOXL 8164.14.00 09/16
05/05/2021 11:07

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:08
02 Std. Sol.	0.297	11:10
03 Room Air	0.000	11:11
04 Std. Sol.	0.298	11:12
05 Room Air	0.000	11:12
06 Std. Sol.	0.297	11:13
07 Room Air	0.000	11:14

08 Sim Temp = 34.0°C

Simul Ser No = MP5317

Std Sol No = 202012A

County = 08

Oper No. = 666666



Operator Signature

CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006673
Location = TOXL 8164.14.00 09/16
05/05/2021 11:15

Test	AC	Time
01 Room Air	0.000	11:16
02 *Subject Test	INT*	11:17
03 Room Air	0.000	11:17

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

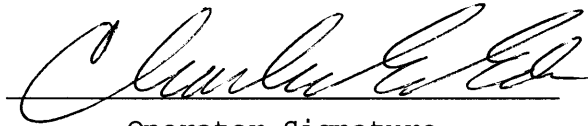

Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10 AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006673
Location = TOXL 8164.14.00 09/16
05/05/2021 11:19

Test	AC	Time
01 Diagnostic	OK	11:19
02 Room Air	0.000	11:20
03 *Subject Test	RFI*	11:20
04 Room Air	0.000	11:21

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS871456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006673
Location = TOXL 8164.14.00 09/16
05/05/2021 11:21

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:21
02 Std. Gas	0.082	11:22
03 Room Air	0.000	11:22
04 Std. Gas	0.082	11:23
05 Room Air	0.000	11:23
06 Std. Gas	0.082	11:24
07 Room Air	0.000	11:24

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

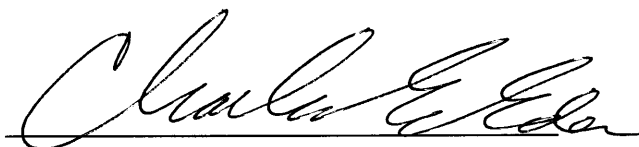

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006673
Location = TOXL 8164.14.00 09/16
05/05/2021 11:25

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:25
02 Std. Gas	0.082	11:26
03 Room Air	0.000	11:26
04 Std. Gas	0.082	11:27
05 Room Air	0.000	11:27
06 Std. Gas	0.082	11:28
07 Room Air	0.000	11:28


Lot No = 02621080A1

Cyl No = 25

Exp Date = 03/05/2023

County = 08

Oper No. = 666666

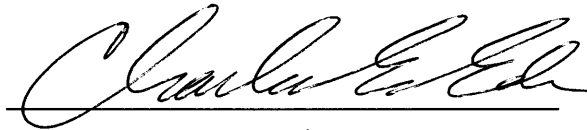

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006673
Location = TOXL 8164.14.00 09/16
05/05/2021 11:28

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:29
02 Std. Gas	0.082	11:29
03 Room Air	0.000	11:30
04 Std. Gas	0.081	11:30
05 Room Air	0.000	11:31
06 Std. Gas	0.081	11:31
07 Room Air	0.000	11:31

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

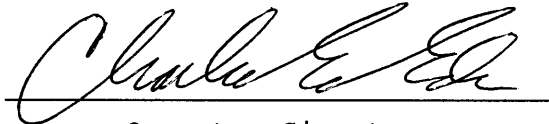

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000