

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006687 Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 1002 psi Regulator: 1000 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.030 AC
Sim. Ser #: MP5289 Lot #: 201911E Exp. Date: 11.19.21
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.400 AC
Sim. Ser #: MP3062 Lot #: 202103E Exp. Date: 3.24.23

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3877 Lot #: ICS6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 05620080A1 Cyl #: 48 Exp. Date: 4.5.22

Test 1	<u>0.082</u>	Test 4	<u>0.082</u>	Test 7	<u>0.082</u>
Test 2	<u>0.081</u>	Test 5	<u>0.082</u>	Test 8	<u>0.082</u>
Test 3	<u>0.082</u>	Test 6	<u>0.083</u>	Test 9	<u>0.082</u>
Average	<u>0.082</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Edr
Breath Analyst Signature

5.5.2021
Date

Kali L. Hieb
Reviewed by

5-11-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
05/05/2021 10:35

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMN OPQRSTUVWXYZ!@# \$%^ &* () _ + ?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMN OPQRSTUVWXYZ!@# \$%^ &* () _ + ?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 02621080A1
Standard Cyl #? 28
Standard Expiration? 03/05/2023
Oper No? 666666

Flow Cal. Date: 10/05/2018
Slope 696
Intercept -609977

IR Calibration Date: 10/05/2018
 3um 9um

0th Coef(*100): -11478 -18771
1st Coef(*100): 255256 132135
2nd Coef(*100): 4432 1676
H2O adj(mg/l*10k): 604 575

***** Printer Test End *****

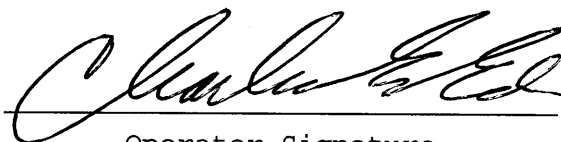

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
05/05/2021 11:00

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:00
02 Std. Sol.	0.029	11:01
03 Room Air	0.000	11:02
04 Std. Sol.	0.029	11:02
05 Room Air	0.000	11:03
06 Std. Sol.	0.030	11:04
07 Room Air	0.000	11:04

08 Sim Temp = 34.0°C

Simul Ser No = MP5289
Std Sol No = 201911E
County = 08 Oper No. = 666666

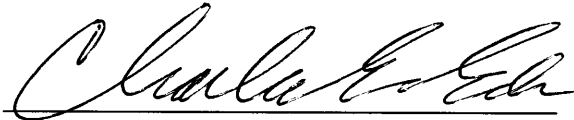

Operator Signature
CHARLES EDER

Remarks:

Low AC
0.030 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
05/05/2021 11:05

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:06
02 Std. Sol.	0.395	11:07
03 Room Air	0.000	11:07
04 Std. Sol.	0.395	11:08
05 Room Air	0.000	11:09
06 Std. Sol.	0.397	11:09
07 Room Air	0.000	11:10

08 Sim Temp = 34.0°C

Simul Ser No = MP3062

Std Sol No = 2072103E

County = 08

Oper No. = 666666



Operator Signature

CHARLES EDER

Remarks:

HIGH AC
0.400 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
05/05/2021 11:15

Test	AC	Time
01 Room Air	0.000	11:16
02 *Subject Test	INT*	11:17
03 Room Air	0.000	11:17

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS871456
Lot No = 05620080A1
Cyl No = 48
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666

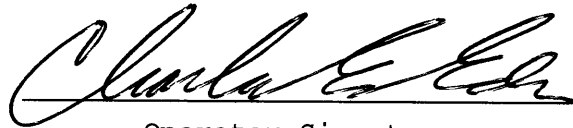

Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
05/05/2021 11:18

Test	AC	Time
01 Diagnostic	OK	11:19
02 Room Air	0.000	11:20
03 *Subject Test	RFI*	11:20
04 Room Air	0.000	11:20

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/08/1987
Sub Sex = Male Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS871456
Lot No = 05620080A1
Cyl No = 48
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

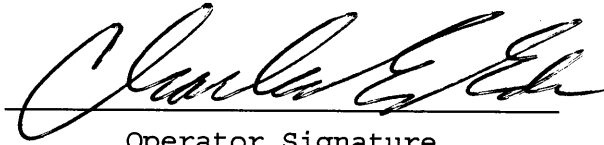

Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
05/05/2021 11:22

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:22
02 Std. Gas	0.082	11:23
03 Room Air	0.000	11:23
04 Std. Gas	0.081	11:23
05 Room Air	0.000	11:24
06 Std. Gas	0.082	11:24
07 Room Air	0.000	11:25

Lot No = 05620080A1
Cyl No = 48
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

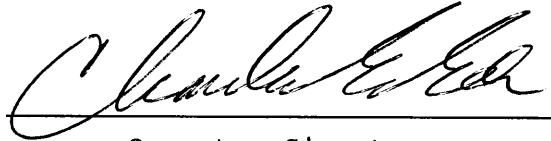

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
05/05/2021 11:25

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:26
02 Std. Gas	0.082	11:26
03 Room Air	0.000	11:27
04 Std. Gas	0.082	11:27
05 Room Air	0.000	11:27
06 Std. Gas	0.083	11:28
07 Room Air	0.000	11:28

Lot No = 05620080A1
Cyl No = 48
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

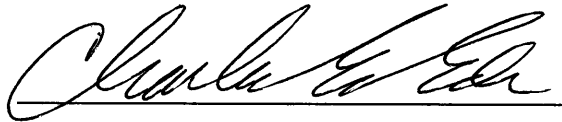

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006687
Location = TOXL 8164.14.00 09/16
05/05/2021 11:29

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:29
02 Std. Gas	0.082	11:29
03 Room Air	0.000	11:30
04 Std. Gas	0.082	11:30
05 Room Air	0.000	11:31
06 Std. Gas	0.082	11:31
07 Room Air	0.000	11:32

Lot No = 05620080A1
Cyl No = 48
Exp Date = 04/05/2022
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000