

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006685 Location: ToxL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 953 psi Regulator: 950 psi

B. Tests (Sign and attach test records):

- Configure simulator for the following tests (Level 1,S).
1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2-13-22
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC ^{CEE}
Sim. Ser #: MP317 Lot #: 20202A Exp. Date: 12-8-22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: JCS6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621080A1 Cyl #: 25 Exp. Date: 3-5-23

Test 1	<u>0.080</u>	Test 4	<u>0.081</u>	Test 7	<u>0.081</u>
Test 2	<u>0.080</u>	Test 5	<u>0.090</u>	Test 8	<u>0.081</u>
Test 3	<u>0.081</u>	Test 6	<u>0.080</u>	Test 9	<u>0.081</u>
Average	<u>0.081</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION, REPLACED SIMULATOR RETURN O-RING, REPLACED EXTERNAL BATTERY

Instrument is acceptable to be used in the field.

Charles E. E
Breath Analyst Signature

5/19/2021
Date

Kali H. Hieb
Reviewed by

5/24/21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006685
Location = TOXL 8164.14.00 09/16
05/19/2021 13:43

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-|=|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-|=|
ABCDEFGHIJKLMNOPQRSTUVWXYZ!@#%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 21
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 09/06/2016
Slope 705
Intercept -687370

IR Calibration Date: 09/06/2016

	3um	9um
0th Coef(*100):	-14155	-22915
1st Coef(*100):	271436	135296
2nd Coef(*100):	2016	1251
H2O adj(mg/l*10k):	372	505

***** Printer Test End *****

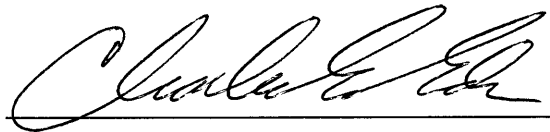

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006685
Location = TOXL 8164.14.00 09/16
05/19/2021 13:49

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:50
02 Std. Sol.	0.018	13:51
03 Room Air	0.000	13:51
04 Std. Sol.	0.018	13:52
05 Room Air	0.000	13:53
06 Std. Sol.	0.018	13:53
07 Room Air	0.000	13:54

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Low Ac
0.020 Ac

Form 106-18000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006685
Location = TOXL 8164.14.00 09/16
05/19/2021 13:55

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:56
02 Std. Sol.	0.302	13:57
03 Room Air	0.000	13:57
04 Std. Sol.	0.302	13:58
05 Room Air	0.000	13:58
06 Std. Sol.	0.301	13:59
07 Room Air	0.000	14:00

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666

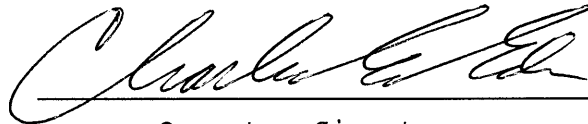

Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006685
Location = TOXL 8164.14.00 09/16
05/19/2021 14:01

Test	AC	Time
01 Room Air	0.000	14:02
02 *Subject Test	INT*	14:03
03 Room Air	0.000	14:03

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS921456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006685
Location = TOXL 8164.14.00 09/16
05/19/2021 14:08

Test	AC	Time
01 Diagnostic	OK	14:09
02 Room Air	0.000	14:10
03 *Subject Test	RFI*	14:10
04 Room Air	0.000	14:10

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS921456
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

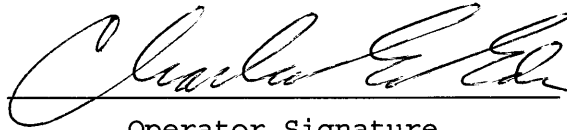

Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006685
Location = TOXL 8164.14.00 09/16
05/19/2021 14:11

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:11
02 Std. Gas	0.080	14:12
03 Room Air	0.000	14:12
04 Std. Gas	0.080	14:13
05 Room Air	0.000	14:13
06 Std. Gas	0.081	14:13
07 Room Air	0.000	14:14

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

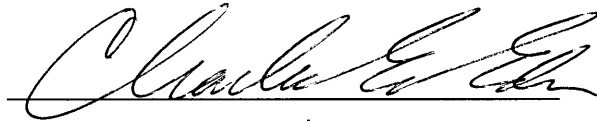

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006685
Location = TOXL 8164.14.00 09/16
05/19/2021 14:14

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:15
02 Std. Gas	0.081	14:15
03 Room Air	0.000	14:16
04 Std. Gas	0.080	14:16
05 Room Air	0.000	14:17
06 Std. Gas	0.080	14:17
07 Room Air	0.000	14:18

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

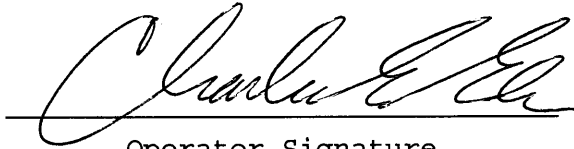

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006685
Location = TOXL 8164.14.00 09/16
05/19/2021 14:18

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:19
02 Std. Gas	0.081	14:19
03 Room Air	0.000	14:19
04 Std. Gas	0.081	14:20
05 Room Air	0.000	14:20
06 Std. Gas	0.081	14:21
07 Room Air	0.000	14:21

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *CALIBRATION CHECK*
0.080 AC

Form 106-I8000