

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006512 Location: TOXL

A. General Setup and Checks:

- 1. Diagnostic Tests Pass and Instrument in Ready Mode
- 2. Breath tube heated
- 3. Date, time and location code (Level 2,E). Re-set if necessary.
- 4. Print test (Level 1,P). Sign and attach test record.
- 5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 202 psi Regulator: 225 psi

B. Tests (Sign and attach test records):

- Configure simulator for the following tests (Level 1,S).
 - 1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2-13-22
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12-8-22

Configure dry gas standard for the following tests (Level 1,S).

- 2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: IC56 Exp. Date: NA
 Display reads "Interferent Detect"
- 3. RFI Check (CMS Mode) Display reads "RFI Detect"
- 4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621080A Cyl #: 25 Exp. Date: 3-5-23

Test 1	<u>0.081</u>	Test 4	<u>0.081</u>	Test 7	<u>0.081</u>
Test 2	<u>0.081</u>	Test 5	<u>0.081</u>	Test 8	<u>0.080</u>
Test 3	<u>0.080</u>	Test 6	<u>0.081</u>	Test 9	<u>0.081</u>
Average	<u>0.081</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION, REPLACED EXTERNAL BATTERY

Instrument is acceptable to be used in the field.

Charles E. Eder
Breath Analyst Signature

5/21/2021
Date

Kali L. Hiet
Reviewed by

5/24/21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006512
Location = TOXL 8164.14.00 09/16
05/21/2021 10:30

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 13
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 08/20/2015
Slope 680
Intercept -660856

IR Calibration Date: 08/21/2015

	3um	9um
0th Coef(*100):	-23051	-19261
1st Coef(*100):	266836	137135
2nd Coef(*100):	3974	1466
H2O adj(mg/l*10k):	785	487

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006512
Location = TOXL 8164.14.00 09/16
05/21/2021 10:59

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:59
02 Std. Sol.	0.018	11:00
03 Room Air	0.000	11:01
04 Std. Sol.	0.018	11:01
05 Room Air	0.000	11:02
06 Std. Sol.	0.018	11:03
07 Room Air	0.000	11:03

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666

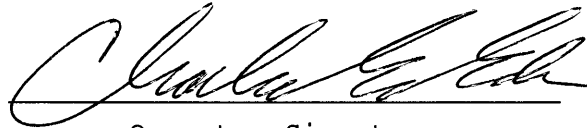

Operator Signature
CHARLES EDER

Remarks:

Low AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006512
Location = TOXL 8164.14.00 09/16
05/21/2021 11:05

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:05
02 Std. Sol.	0.300	11:06
03 Room Air	0.000	11:07
04 Std. Sol.	0.302	11:07
05 Room Air	0.000	11:08
06 Std. Sol.	0.301	11:09
07 Room Air	0.000	11:09

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: HIGH AC
 0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006512
Location = TOXL 8164.14.00 09/16
05/21/2021 11:11

Test	AC	Time
01 Room Air	0.000	11:11
02 *Subject Test	INT*	11:12
03 Room Air	0.000	11:12

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

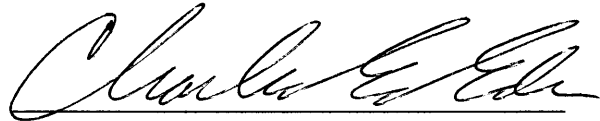

Operator Signature
CHARLES EDER

Remarks: *Interferent Check*

0.10 AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006512
Location = TOXL 8164.14.00 09/16
05/21/2021 11:14

Test	AC	Time
01 Diagnostic	OK	11:14
02 Room Air	0.000	11:15
03 *Subject Test	RFI*	11:15
04 Room Air	0.000	11:16

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 02621080A1
Cyl No = 25
Expiration Date = 03/05/2023
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *RFI CHECK*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006512
Location = TOXL 8164.14.00 09/16
05/21/2021 11:16

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:16
02 Std. Gas	0.081	11:17
03 Room Air	0.000	11:17
04 Std. Gas	0.081	11:18
05 Room Air	0.000	11:18
06 Std. Gas	0.080	11:19
07 Room Air	0.000	11:19

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

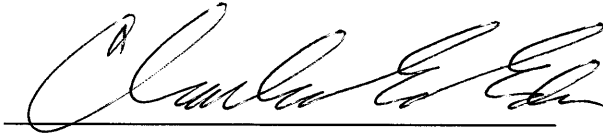

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006512
Location = TOXL 8164.14.00 09/16
05/21/2021 11:20

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:20
02 Std. Gas	0.081	11:21
03 Room Air	0.000	11:21
04 Std. Gas	0.081	11:22
05 Room Air	0.000	11:22
06 Std. Gas	0.081	11:22
07 Room Air	0.000	11:23

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006512
Location = TOXL 8164.14.00 09/16
05/21/2021 11:23

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:24
02 Std. Gas	0.081	11:24
03 Room Air	0.000	11:25
04 Std. Gas	0.080	11:25
05 Room Air	0.000	11:26
06 Std. Gas	0.081	11:26
07 Room Air	0.000	11:27

Lot No = 02621080A1
Cyl No = 25
Exp Date = 03/05/2023
County = 08 Oper No. = 666666

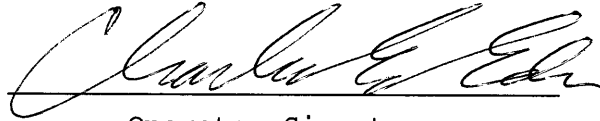

Operator Signature
CHARLES EDER

Remarks: *CALIBRATION CHECK*
0.080 AC

Form 106-I8000