

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006690

Location: TOUL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 1011 psi Regulator: 1000 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check

- a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.015 AC
Sim. Ser #: MP5319 Lot #: 201911C Exp. Date: 11-19-21
- b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.400 AC
Sim. Ser #: MP3060 Lot #: 19108 Exp. Date: 10-20-21

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR7348 Lot #: 1C55 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 02621080A1 Cyl #: 026 Exp. Date: 3-5-23

| | | |
|----------------------|---------------------|---------------------|
| Test 1 <u>0.082</u> | Test 4 <u>0.082</u> | Test 7 <u>0.081</u> |
| Test 2 <u>0.082</u> | Test 5 <u>0.081</u> | Test 8 <u>0.082</u> |
| Test 3 <u>0.081</u> | Test 6 <u>0.082</u> | Test 9 <u>0.081</u> |
| Average <u>0.082</u> | | |

C. Remarks/Maintenance: Annual inspection

Instrument is acceptable to be used in the field.

Kelli G. Hiest
Breath Analyst Signature

5-26-21
Date

Charles E. Ehr
Reviewed by

5-26-2021
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/26/2021 10:43

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 35
Standard Expiration? 11/05/2021
Oper No? 132598

Flow Cal. Date: 08/23/2018
Slope 677
Intercept -593298

IR Calibration Date: 08/23/2018

| | 3um | 9um |
|--------------------|--------|--------|
| 0th Coef(*100): | -8380 | -21663 |
| 1st Coef(*100): | 265142 | 130429 |
| 2nd Coef(*100): | 3933 | 1429 |
| H2O adj(mg/l*10k): | 412 | 539 |

***** Printer Test End *****

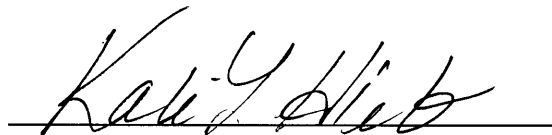

Operator Signature
KALI HIEB

Remarks: *print test*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/26/2021 10:47

WET CAL CHECK

| Test | AC | Time |
|--------------|-------|-------|
| 01 Room Air | 0.000 | 10:48 |
| 02 Std. Sol. | 0.014 | 10:49 |
| 03 Room Air | 0.000 | 10:49 |
| 04 Std. Sol. | 0.014 | 10:50 |
| 05 Room Air | 0.000 | 10:51 |
| 06 Std. Sol. | 0.014 | 10:51 |
| 07 Room Air | 0.000 | 10:52 |

08 Sim Temp = 34.0°C

Simul Ser No = MP5319
Std Sol No = 201911C
County = 08 Oper No. = 132598

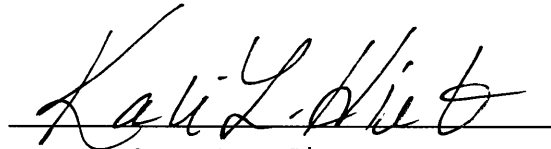
Operator Signature
KALI HIEB

Remarks: *low AC 0.015 AC*
cal check

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/26/2021 10:54

WET CAL CHECK

| Test | AC | Time |
|--------------|-------|-------|
| 01 Room Air | 0.000 | 10:55 |
| 02 Std. Sol. | 0.400 | 10:56 |
| 03 Room Air | 0.000 | 10:56 |
| 04 Std. Sol. | 0.406 | 10:57 |
| 05 Room Air | 0.000 | 10:58 |
| 06 Std. Sol. | 0.406 | 10:58 |
| 07 Room Air | 0.000 | 10:59 |

08 Sim Temp = 33.9°C

Simul Ser No = MP3060
Std Sol No = 19108
County = 08 Oper No. = 132598

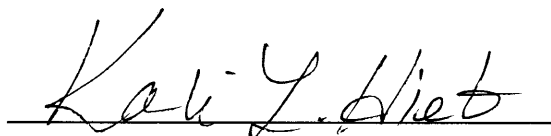

Operator Signature
KALI HIEB

Remarks: *High cal check 0.400 AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/26/2021 11:02

| Test | AC | Time |
|------------------|-------|-------|
| 01 Room Air | 0.000 | 11:03 |
| 02 *Subject Test | INT* | 11:03 |
| 03 Room Air | 0.000 | 11:04 |

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

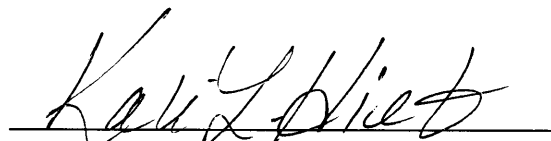

Operator Signature
KALI HIEB

Remarks: *Interferent check*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/26/2021 11:05

| Test | AC | Time |
|---------------|-------|-------|
| 01 Diagnostic | OK | 11:06 |
| 02 Room Air | 0.000 | 11:06 |
| 03 Reference | RFI* | 11:06 |
| 04 Room Air | 0.000 | 11:07 |

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 02621080A1
Cyl No = 26
Expiration Date = 03/05/2023
County = 08 Oper No. = 132598

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

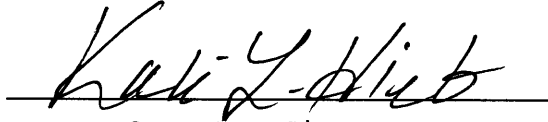
Operator Signature
KALI HIEB

Remarks: *RFI Check*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/26/2021 11:08

DRY CAL CHECK

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 11:08 |
| 02 Std. Gas | 0.082 | 11:08 |
| 03 Room Air | 0.000 | 11:09 |
| 04 Std. Gas | 0.082 | 11:09 |
| 05 Room Air | 0.000 | 11:10 |
| 06 Std. Gas | 0.081 | 11:10 |
| 07 Room Air | 0.000 | 11:11 |

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

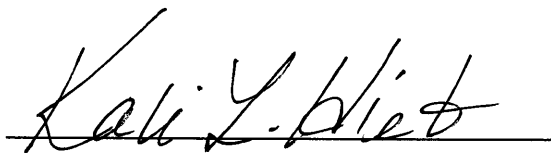

Operator Signature
KALI HIEB

Remarks: *cal check 0.080AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/26/2021 11:14

DRY CAL CHECK

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 11:14 |
| 02 Std. Gas | 0.082 | 11:14 |
| 03 Room Air | 0.000 | 11:15 |
| 04 Std. Gas | 0.081 | 11:15 |
| 05 Room Air | 0.000 | 11:16 |
| 06 Std. Gas | 0.082 | 11:16 |
| 07 Room Air | 0.000 | 11:17 |

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

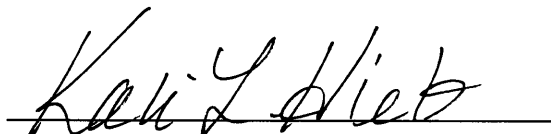
Operator Signature
KALI HIEB

Remarks: *cal check 0.000 AC*

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006690
Location = TOXL 8164.14.00 09/16
05/26/2021 11:17

DRY CAL CHECK

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 11:18 |
| 02 Std. Gas | 0.081 | 11:18 |
| 03 Room Air | 0.000 | 11:18 |
| 04 Std. Gas | 0.082 | 11:19 |
| 05 Room Air | 0.000 | 11:19 |
| 06 Std. Gas | 0.081 | 11:20 |
| 07 Room Air | 0.000 | 11:20 |

Lot No = 02621080A1
Cyl No = 26
Exp Date = 03/05/2023
County = 08 Oper No. = 132598

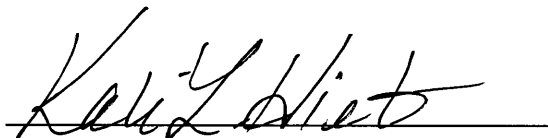
Operator Signature
KALI HIEB

Remarks: *cal check O.CBDAC*

Form 106-I8000