

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006507

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 215 psi Regulator: 250 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICSC Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 05620 080A1 Cyl #: 6 Exp. Date: 4.5.22

Test 1	<u>0.080</u>	Test 4	<u>0.080</u>	Test 7	<u>0.080</u>
Test 2	<u>0.079</u>	Test 5	<u>0.080</u>	Test 8	<u>0.080</u>
Test 3	<u>0.080</u>	Test 6	<u>0.080</u>	Test 9	<u>0.080</u>
Average	<u>0.080</u>				

C. Remarks/Maintenance: ANNUAL INSPECTION

Instrument is acceptable to be used in the field.

Charles E. Ehr
Breath Analyst Signature

6/3/21
Date

Kali Y. D'Ho
Reviewed by

6-7-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006507
Location = TOXL 8164.14.00 09/16
06/03/2021 10:52

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 24119080A1
Standard Cyl #? 36
Standard Expiration? 11/05/2021
Oper No? 666666

Flow Cal. Date: 08/20/2015
Slope 659
Intercept -658315

IR Calibration Date: 08/20/2015

	3um	9um
0th Coef (*100):	-9452	-11722
1st Coef (*100):	258808	139588
2nd Coef (*100):	4476	1674
H2O adj (mg/l*10k):	499	376

***** Printer Test End *****

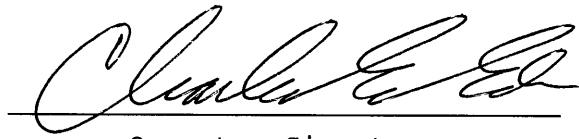

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006507
Location = TOXL 8164.14.00 09/16
06/03/2021 10:58

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:58
02 Std. Sol.	0.018	10:59
03 Room Air	0.000	10:59
04 Std. Sol.	0.018	11:00
05 Room Air	0.000	11:01
06 Std. Sol.	0.019	11:01
07 Room Air	0.000	11:02

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Low AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006507
Location = TOXL 8164.14.00 09/16
06/03/2021 11:06

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:07
02 Std. Sol.	0.300	11:08
03 Room Air	0.000	11:08
04 Std. Sol.	0.300	11:09
05 Room Air	0.000	11:09
06 Std. Sol.	0.301	11:10
07 Room Air	0.000	11:11

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006507
Location = TOXL 8164.14.00 09/16
06/03/2021 11:12

Test	AC	Time
01 Room Air	0.000	11:13
02 *Subject Test	INT*	11:14
03 Room Air	0.000	11:15

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS921456
Lot No = 05620080A1
Cyl No = 6
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10 AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006507
Location = TOXL 8164.14.00 09/16
06/03/2021 11:16

Test	AC	Time
01 Diagnostic	OK	11:17
02 Room Air	0.000	11:17
03 *Subject Test	RFI*	11:18
04 Room Air	0.000	11:18

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 02/01/1992
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS921456
Lot No = 05620080A1
Cyl No = 6
Expiration Date = 04/05/2022
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *RFI CHECK*

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006507
Location = TOXL 8164.14.00 09/16
06/03/2021 11:18

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:19
02 Std. Gas	0.080	11:19
03 Room Air	0.000	11:20
04 Std. Gas	0.079	11:20
05 Room Air	0.000	11:21
06 Std. Gas	0.080	11:21
07 Room Air	0.000	11:21


Lot No = 05620080A1

Cyl No = 6

Exp Date = 04/05/2022

County = 08

Oper No. = 666666

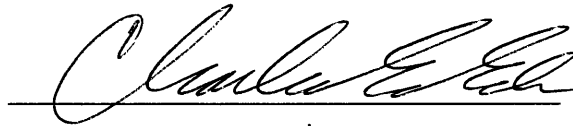

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006507
Location = TOXL 8164.14.00 09/16
06/03/2021 11:22

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:23
02 Std. Gas	0.080	11:23
03 Room Air	0.000	11:23
04 Std. Gas	0.080	11:24
05 Room Air	0.000	11:24
06 Std. Gas	0.080	11:25
07 Room Air	0.000	11:25

Lot No = 05620080A1
Cyl No = 6
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

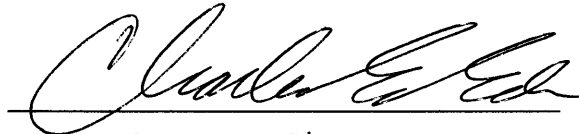

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006507
Location = TOXL 8164.14.00 09/16
06/03/2021 11:26

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:26
02 Std. Gas	0.080	11:27
03 Room Air	0.000	11:27
04 Std. Gas	0.080	11:27
05 Room Air	0.000	11:28
06 Std. Gas	0.080	11:28
07 Room Air	0.000	11:29

Lot No = 05620080A1
Cyl No = 6
Exp Date = 04/05/2022
County = 08 Oper No. = 666666

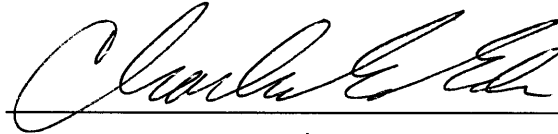

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000