

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006681

Location: TOXL

A. General Setup and Checks:

1. Diagnostic Tests Pass and Instrument in Ready Mode
2. Breath tube heated
3. Date, time and location code (Level 2,E). Re-set if necessary.
4. Print test (Level 1,P). Sign and attach test record.
5. Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
 - a. Display: 934 psi Regulator: 900 psi

B. Tests (Sign and attach test records):

Configure simulator for the following tests (Level 1,S).

1. Wet Calibration Check
 - a. Low AC (Level 1,C): Known Value ≤ 0.03 AC: 0.020 AC
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
 - b. High AC (Level 1,C): Known Value ≥ 0.25 AC: 0.300 AC
Sim. Ser #: MP5317 Lot #: 202012A Exp. Date: 12.8.22

Configure dry gas standard for the following tests (Level 1,S).

2. Interferent Check (Level 1,B): Known Value: 0.10 AC + 0.05% Acetone
Sim. Ser #: DR3847 Lot #: ICS 6 Exp. Date: NA
 Display reads "Interferent Detect"
3. RFI Check (CMS Mode) Display reads "RFI Detect"
4. Dry Calibration Check (Level 1,C): Known Value 0.080 AC
Gas Cyl Lot #: 24119080A1 Cyl #: 31 Exp. Date: 11.5.21

Test 1 <u>0.078</u>	Test 4 <u>0.079</u>	Test 7 <u>0.079</u>
Test 2 <u>0.079</u>	Test 5 <u>0.079</u>	Test 8 <u>0.079</u>
Test 3 <u>0.078</u>	Test 6 <u>0.079</u>	Test 9 <u>0.078</u>
Average <u>0.079</u>		

C. Remarks/Maintenance: ANNUAL INSPECTION, REPLACED SIMULATOR RETURN O-RING

Instrument is acceptable to be used in the field.

Charles E. Ehr
Breath Analyst Signature

6/3/21
Date

Kali G. Ditt
Reviewed by

6-7-21
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006681
Location = TOXL 8164.14.00 09/16
06/03/2021 14:47

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup

Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 05620080A1
Standard Cyl #? 42
Standard Expiration? 04/05/2022
Oper No? 666666

Flow Cal. Date: 05/27/2020
Slope 651
Intercept -622365

IR Calibration Date: 05/27/2020

	3um	9um
0th Coef(*100):	-10420	-19573
1st Coef(*100):	269401	137403
2nd Coef(*100):	1095	923
H2O adj(mg/l*10k):	127	287

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006681
Location = TOXL 8164.14.00 09/16
06/03/2021 14:52

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:52
02 Std. Sol.	0.018	14:53
03 Room Air	0.000	14:53
04 Std. Sol.	0.019	14:54
05 Room Air	0.000	14:55
06 Std. Sol.	0.019	14:55
07 Room Air	0.000	14:56

08 Sim Temp = 34.0°C

Simul Ser No = MP3064
Std Sol No = 20070
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Low AC*
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006681
Location = TOXL 8164.14.00 09/16
06/03/2021 14:57

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:58
02 Std. Sol.	0.300	14:59
03 Room Air	0.000	14:59
04 Std. Sol.	0.300	15:00
05 Room Air	0.000	15:00
06 Std. Sol.	0.299	15:01
07 Room Air	0.000	15:02

08 Sim Temp = 34.0°C

Simul Ser No = MP5317
Std Sol No = 202012A
County = 08 Oper No. = 666666

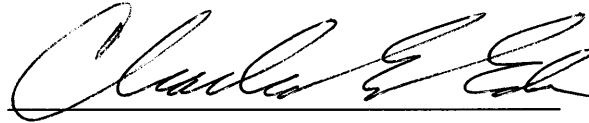

Operator Signature

CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006681
Location = TOXL 8164.14.00 09/16
06/03/2021 15:04

Test	AC	Time
01 Room Air	0.000	15:05
02 *Subject Test	INT*	15:05
03 Room Air	0.000	15:06

*Invalid Test
Interferent Detected

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 31
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

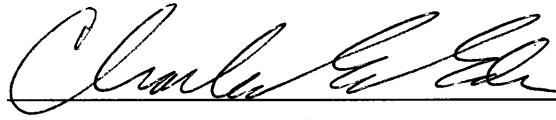

Operator Signature
CHARLES EDER

Remarks: *Interferent Check*
0.10AC + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006681
Location = TOXL 8164.14.00 09/16
06/03/2021 15:06

Test	AC	Time
01 Diagnostic	OK	15:07
02 Room Air	0.000	15:07
03 *Subject Test	RFI*	15:07
04 Room Air	0.000	15:08

*Invalid Test
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE
Sub DOB = 07/25/1998
Sub Sex = Male Weight = NA
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/TES989643
Lot No = 24119080A1
Cyl No = 31
Expiration Date = 11/05/2021
County = 08 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006681
Location = TOXL 8164.14.00 09/16
06/03/2021 15:10

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:10
02 Std. Gas	0.078	15:11
03 Room Air	0.000	15:11
04 Std. Gas	0.079	15:12
05 Room Air	0.000	15:12
06 Std. Gas	0.078	15:12
07 Room Air	0.000	15:13

Lot No = 24119080A1
Cyl No = 31
Exp Date = 11/05/2021
County = 08 Oper No. = 666666

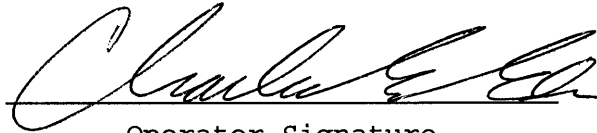

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006681
Location = TOXL 8164.14.00 09/16
06/03/2021 15:14

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:14
02 Std. Gas	0.079	15:15
03 Room Air	0.000	15:15
04 Std. Gas	0.079	15:16
05 Room Air	0.000	15:16
06 Std. Gas	0.079	15:16
07 Room Air	0.000	15:17

Lot No = 24119080A1
Cyl No = 31
Exp Date = 11/05/2021
County = 08 Oper No. = 666666

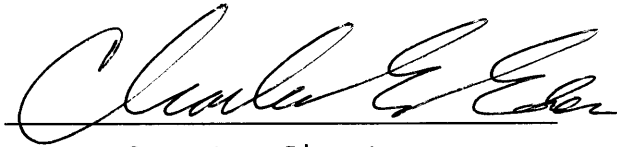

Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006681
Location = TOXL 8164.14.00 09/16
06/03/2021 15:17

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:18
02 Std. Gas	0.079	15:18
03 Room Air	0.000	15:19
04 Std. Gas	0.079	15:19
05 Room Air	0.000	15:20
06 Std. Gas	0.078	15:20
07 Room Air	0.000	15:20

Lot No = 24119080A1
Cyl No = 31
Exp Date = 11/05/2021
County = 08 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

CALIBRATION CHECK
0.080 AC

Form 106-I8000