

INTOXILYZER® 8000 INSPECTION

Intoxilyzer® 8000 Serial Number: 80-006679 Location: TOXL

A. General Setup and Checks:

1.  Diagnostic Tests Pass and Instrument in Ready Mode
2.  Breath tube heated
3.  Date, time and location code (Level 2,E). Re-set if necessary.
4.  Print test (Level 1,P). Sign and attach test record.
5.  Tank monitor (Level 3,D,G). Display and Regulator within 50 psi.
  - a. Display: 997 psi Regulator: 1000 psi

B. Tests (Sign and attach test records):

- Configure simulator for the following tests (Level 1,S).
1. Wet Calibration Check
    - a.  Low AC (Level 1,C): Known Value  $\leq 0.03$  AC: 0.020 AC  
Sim. Ser #: MP3064 Lot #: 20070 Exp. Date: 2.13.22
    - b.  High AC (Level 1,C): Known Value  $\geq 0.25$  AC: 0.300 AC  
Sim. Ser #: MP5317 Lot #: 202001B Exp. Date: 1.28.22

Configure dry gas standard for the following tests (Level 1,S).

2.  Interferent Check (Level 1,B): Known Value: 0.10AC + 0.05% Acetone  
Sim. Ser #: DR3847 Lot #: ICSG Exp. Date: NA  
 Display reads "Interferent Detect"
3.  RFI Check (CMS Mode)  Display reads "RFI Detect"
4.  Dry Calibration Check (Level 1,C): Known Value 0.080 AC  
Gas Cyl Lot #: 24119080A1 Cyl #: 5 Exp. Date: 11.5.21

Test 1 <u>0.080</u>	Test 4 <u>0.081</u>	Test 7 <u>0.080</u>
Test 2 <u>0.081</u>	Test 5 <u>0.081</u>	Test 8 <u>0.080</u>
Test 3 <u>0.080</u>	Test 6 <u>0.080</u>	Test 9 <u>0.081</u>
Average <u>0.080</u>		

C. Remarks/Maintenance: ANNUAL INSPECTION PERFORMED  
TANK SENSOR CALIBRATION, REPLACED EXTERNAL  
BATTERY

Instrument is acceptable to be used in the field.

[Signature]  
Breath Analyst Signature

6/23/21  
Date

[Signature]  
Reviewed by

6-28-21  
Date

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006679  
Location = TOXL                    8164.14.00 09/16  
06/23/2021                            13:47

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&\*()\_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&\*()\_+?

Current Instrument Setup

Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?          1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            02621080A1  
Standard Cyl #?            36  
Standard Expiration?        03/05/2023  
Oper No?                    666666

Flow Cal. Date:            09/06/2016  
Slope                        701  
Intercept                    -682926

IR Calibration Date:        09/06/2016

	3um	9um
0th Coef(*100):	-18983	-23165
1st Coef(*100):	280986	134481
2nd Coef(*100):	2443	1290
H2O adj(mg/l*10k):	569	553

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
CHARLES EDER

Remarks:

PRINT TEST

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006679  
Location = TOXL                    8164.14.00 09/16  
06/23/2021                            13:57

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:57
02 Std. Sol.	0.018	13:58
03 Room Air	0.000	13:59
04 Std. Sol.	0.018	14:00
05 Room Air	0.000	14:00
06 Std. Sol.	0.018	14:01
07 Room Air	0.000	14:01

08 Sim Temp = 34.0°C

Simul Ser No = MP3064  
Std Sol No = 20070  
County = 08                            Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks:

*LOW AC*  
*0.020 AC*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006679  
Location = TOXL      8164.14.00 09/16  
06/23/2021      14:08

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:08
02 Std. Sol.	0.293	14:09
03 Room Air	0.000	14:10
04 Std. Sol.	0.294	14:10
05 Room Air	0.000	14:11
06 Std. Sol.	0.294	14:12
07 Room Air	0.000	14:12

08 Sim Temp = 34.0°C

Simul Ser No = MP5317  
Std Sol No = 202001B  
County = 08      Oper No. = 666666

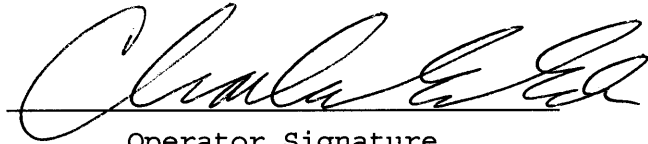

Operator Signature  
CHARLES EDER

Remarks: HIGH AC  
0.300 AC

Form 106-18000


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006679  
Location = TOXL      8164.14.00 09/16  
06/23/2021      14:13

Test	AC	Time
01 Room Air	0.000	14:14
02 *Subject Test	INT*	14:15
03 Room Air	0.000	14:15

\*Invalid Test  
Interferent Detected

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male      Weight = NA  
Test = DUI      Cit = INTERFERENT  
Dr. Lic. = ND/TES989643  
Lot No = 24119080A1  
Cyl No = 5  
Expiration Date = 11/05/2021  
County = 08      Oper No. = 666666

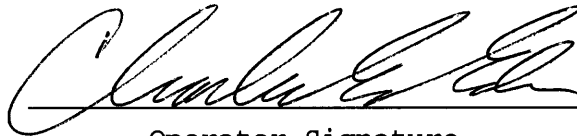

Operator Signature  
CHARLES EDER

Remarks:

*Interferent Check*  
*0.10AC + 0.05% ACETONE*

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006679  
Location = TOXL                 8164.14.00 09/16  
06/23/2021                        14:16

Test	AC	Time
01 Diagnostic	OK	14:16
02 Room Air	0.000	14:17
03 *Subject Test	RFI*	14:17
04 Room Air	0.000	14:17

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, DONOR2 NONE  
Sub DOB = 07/25/1998  
Sub Sex = Male                     Weight = NA  
Test = DUI                         Cit = RFI CHECK  
Dr. Lic. = ND/TES989643  
Lot No = 24119080A1  
Cyl No = 5  
Expiration Date = 11/05/2021  
County = 08                        Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

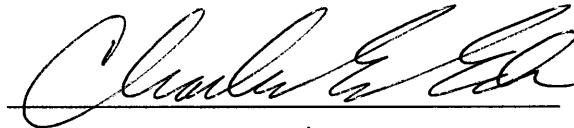

Operator Signature  
CHARLES EDER

Remarks:

RFI CHECK

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006679  
Location = TOXL      8164.14.00 09/16  
06/23/2021      14:18

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:18
02 Std. Gas	0.080	14:19
03 Room Air	0.000	14:19
04 Std. Gas	0.081	14:19
05 Room Air	0.000	14:20
06 Std. Gas	0.080	14:20
07 Room Air	0.000	14:21

Lot No = 24119080A1  
Cyl No = 5  
Exp Date = 11/05/2021  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006679  
Location = TOXL      8164.14.00 09/16  
06/23/2021      14:21

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:21
02 Std. Gas	0.081	14:22
03 Room Air	0.000	14:22
04 Std. Gas	0.081	14:23
05 Room Air	0.000	14:23
06 Std. Gas	0.080	14:24
07 Room Air	0.000	14:24

Lot No = 24119080A1  
Cyl No = 5  
Exp Date = 11/05/2021  
County = 08      Oper No. = 666666



Operator Signature  
CHARLES EDER

Remarks: CALIBRATION CHECK  
0.080 AC

Form 106-I8000



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006679  
Location = TOXL      8164.14.00 09/16  
06/23/2021      14:24

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:25
02 Std. Gas	0.080	14:25
03 Room Air	0.000	14:26
04 Std. Gas	0.080	14:26
05 Room Air	0.000	14:27
06 Std. Gas	0.081	14:27
07 Room Air	0.000	14:27


Lot No = 24119080A1

Cyl No = 5

Exp Date = 11/05/2021

County = 08

Oper No. = 666666

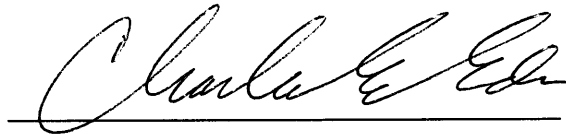

Operator Signature  
CHARLES EDER

Remarks:

CALIBRATION CHECK  
0.080 AC

Form 106-I8000