



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM
 SFN 59281 (06/2018)

Serial Number	16021080A1 ^{SP} 80-006676	Instrument Location	Mountaintrail Co Booking
Reason for Install/Repair			
<input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____			

Check When Done:

- 1. Surge Protector Installed/Property Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. Radio Frequency Interference (RFI) Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if any): _____
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN504096, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature	<i>Shayla Rodgers 4477</i>	Date	6/28/22
---------------------------	----------------------------	------	---------

Crime Laboratory Use Only

This installation has been reviewed and the instrument is approved to be used for the analysis of breath to determine alcohol concentration from the date the Field Inspector performed the installation. This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Reviewed/Certified By	<i>Janelle Pertschiller</i>	Certified Date	7/11/2022
-----------------------	-----------------------------	----------------	-----------

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006676
Location = MOSO 8164.14.00 09/16
06/28/2022 18:09

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	18:10
02 Std. Gas	0.081	18:10
03 Room Air	0.000	18:10
04 Std. Gas	0.080	18:11
05 Room Air	0.000	18:11
06 Std. Gas	0.080	18:12
07 Room Air	0.000	18:12

Lot No = 26021080A1
Cyl No = 016
Exp Date = 10/05/2023
County = 31 Oper No. = 132957


Operator Signature
SHAYLA RODGERS

Remarks:

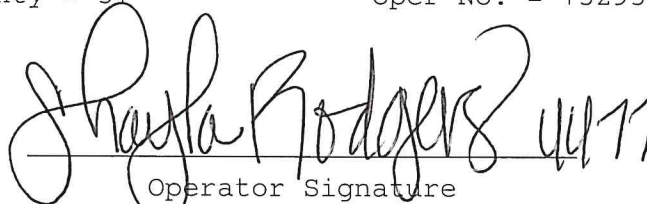
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-006676
Location = MOSO 8164.14.00 09/16
06/28/2022 18:14

Test	AC	Time
01 Room Air	0.000	18:17
02 *Subject Test	RFI*	18:17
03 Room Air	0.000	18:17

*Invalid Test
Inhibited - RFI

Sub Name = DOE, JOHN L
Sub DOB = 01/01/1900
Sub Sex = Male Weight = 110
Test = DUI Cit = 00000000
Dr. Lic. = ND/0000000
Lot No = 26021080A1
Cyl No = 016
Expiration Date = 10/05/2023
County = 31 Oper No. = 132957


Operator Signature
SHAYLA RODGERS

Remarks: