





**ETHANOL GAS STANDARD CYLINDER REPORT**  
 NORTH DAKOTA OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION-TOXICOLOGY SECTION/BREATH ALCOHOL PROGRAM  
 SFN 59282 (08/2018)

Chemical Test Operator Name (Print) CHRISTOPHER L. ALMLIE		
Location BURKE COUNTY SHERIFF'S SHOP		Intoxilyzer® Serial Number 80-006673
Gas Lot Number 34921080A1	Gas Cylinder Number 54	Gas Expiration Date 02/05/2024

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).  
 Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
  - A. 0.0 81 AC
  - B. 0.0 8 L AC
  - C. 00 71 AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
  - A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).
  - B. ACA Test Record.

Chemical Test Operator Signature  #4172	Date 4/9/2022
Reviewed By (Crime Laboratory Use Only) 	Date 22 Apr 22

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

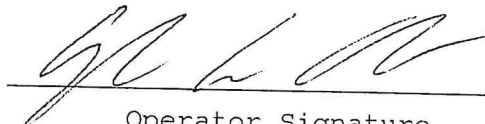
CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006673  
Location = BURK      8164.14.00 09/16  
04/09/2022      15:12

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:17
02 Std. Gas	0.081	15:17
03 Room Air	0.000	15:18
04 Std. Gas	0.081	15:18
05 Room Air	0.000	15:19
06 Std. Gas	0.079	15:19
07 Room Air	0.000	15:19

Lot No = 34921080A1  
Cyl No = 54  
Exp Date = 02/05/2024  
County = 07

Oper No. = 132664

 #4172  
Operator Signature  
CHRISTOPHER ALMLIE

Remarks: