



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Tyler Wolfe</u>		
Location: <u>HARV</u>		
Intoxilyzer® Serial Number: <u>80-SN-004935</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>31</u>	Expiration Date: <u>12/23/2011</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>077</u> %		
Test 2: 0. <u>078</u> %		
Test 3: 0. <u>078</u> %		
(ATTACH TEST RECORD)		

Tyler Wolfe
Chemical Test Operator Signature

01/03/11
Date

Deb Kashur
Reviewed By

10 Jan 2011
Date


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004935
Location = HARV 8164.13.00 06/09
01/03/2011 21:02

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	21:02
02 Std. Gas	0.077	21:03
03 Room Air	0.000	21:03
04 Std. Gas	0.078	21:04
05 Room Air	0.000	21:04
06 Std. Gas	0.078	21:04
07 Room Air	0.000	21:05

Lot No = 709352
Cyl No = 31
Exp Date = 12/23/2011
County = 52 Oper No. = 060901

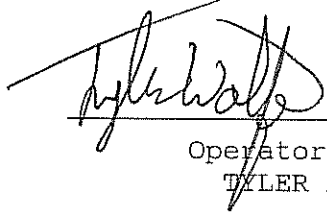

Operator Signature
TYLER A. WOLFE

Remarks:

ACA

Form 106-I8000

80-004935
P. 67 of 67
JAM