



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Adam Krabbenhaft</u>		
Location: <u>Lamoure County Sheriff's office</u>		
Intoxilyzer® Serial Number: <u>80-004942</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>14</u>	Expiration Date: <u>12-23-11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>080</u> %		
Test 2: 0. <u>081</u> %		
Test 3: 0. <u>080</u> %		
(ATTACH TEST RECORD)		

Adam Krabbenhaft
Chemical Test Operator Signature

1-4-11
Date

Deb Kashner
Reviewed By

10 Jan 2011
Date

80-004942
P. 57 of 58
SFN


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004942
Location = LAMO 8164.13.00 06/09
01/04/2011 14:04

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:05
02 Std. Gas	0.080	14:05
03 Room Air	0.000	14:06
04 Std. Gas	0.081	14:06
05 Room Air	0.000	14:07
06 Std. Gas	0.080	14:07
07 Room Air	0.000	14:07

Lot No = 709352
Cyl No = 14
Exp Date = 12/23/2011
County = 23 Oper No. = 020828

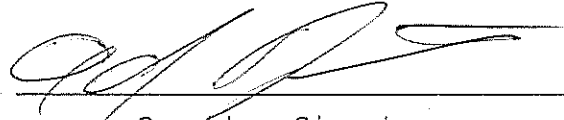

Operator Signature
ADAM R. KRABBENHOFT

Remarks:

ACA TEST

Form 106-I8000

80-004942
P. 58 of 58
km