



# ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Chris Pulver</u>		
Location: <u>Mountainail SO</u>		
Intoxilyzer® Serial Number: <u>80-004943</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>34</u>	Expiration Date: <u>12-23-11</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: <u>0.080</u> %		
Test 2: <u>0.081</u> %		
Test 3: <u>0.080</u> %		
(ATTACH TEST RECORD)		

Chris Pulver  
Chemical Test Operator Signature

1-7-11  
Date

Deb Kashner  
Reviewed By

12 Jan 2011  
Date

80-004943  
P. 61 of 62  
jm


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004943  
Location = STAN      8164.13.00 06/09  
01/07/2011      21:41

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	21:43
02 Std. Gas	0.080	21:43
03 Room Air	0.000	21:44
04 Std. Gas	0.081	21:44
05 Room Air	0.000	21:44
06 Std. Gas	0.080	21:45
07 Room Air	0.000	21:45

Lot No = 709352  
Cyl No = 34  
Exp Date = 12/23/2011  
County = 31      Oper No. = 049912

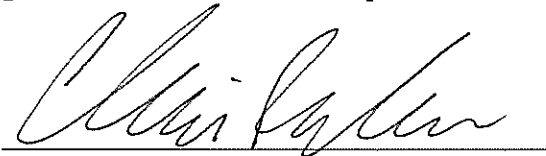

Operator Signature  
CHRISTOPHER PULVER

Remarks:

Form 106-I8000

80-004943  
P. 62 of 62  
JFM