



ETHANOL BREATH STANDARD CYLINDER REPORT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59282 (5-2011)

Chemical Test Operator Name (Print) <u>Robert Kennedy</u>		
Location <u>Rugby</u>	Intoxilyzer® Serial Number <u>80-004203</u>	
Gas Lot Number <u>14214080A6</u>	Gas Cylinder Number <u>56</u>	Gas Expiration Date <u>7/5/2016</u>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).

Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).

- A. 0.084 AC
- B. 0.083 AC
- C. 0.084 AC

- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 - A. Ethanol Breath Standard Cylinder Report (SFN59282, Form 105-G).
 - B. ACA Test Record.

Chemical Test Operator Signature <u>[Signature]</u>	Date <u>1/9/2016</u> ²⁰¹⁵ ^{DK}
Reviewed By (Crime Laboratory Use Only) <u>[Signature]</u>	Date <u>20 Jan 2015</u>


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004203
Location = RUGB 8164.13.00 06/09
01/09/2015 15:55

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:56
02 Std. Gas	0.084	15:57
03 Room Air	0.000	15:57
04 Std. Gas	0.083	15:58
05 Room Air	0.000	15:58
06 Std. Gas	0.084	15:59
07 Room Air	0.000	15:59

Lot No = 14214080A6
Cyl No = 56
Exp Date = 07/05/2016
County = 35 Oper No. = 069108

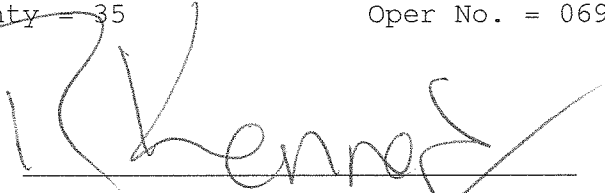

Operator Signature
ROBERT KENNEDY

Remarks: